




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031594.D
Acq On : 27 Jan 2025 15:41
Operator : SY/MD
Sample : Q1190-02
Misc : 14.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:25:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

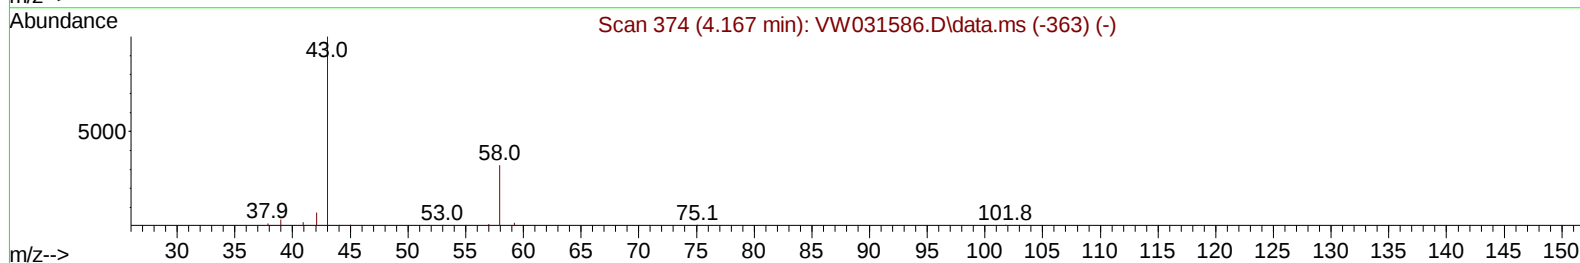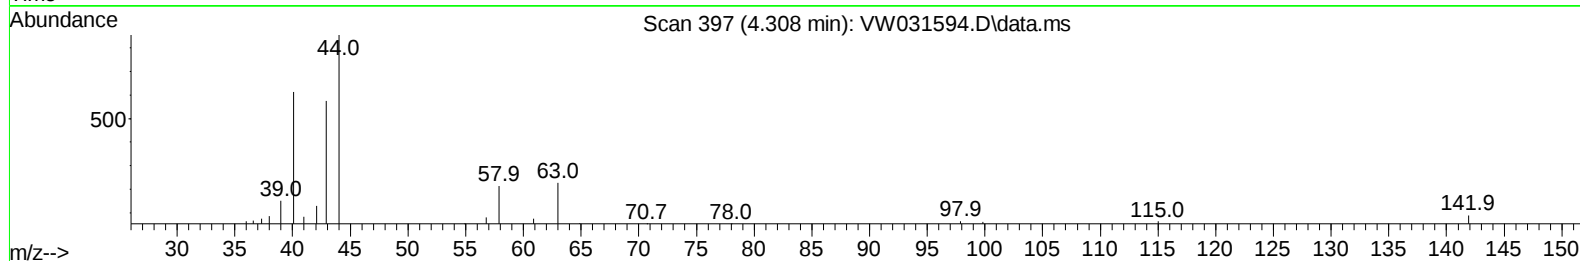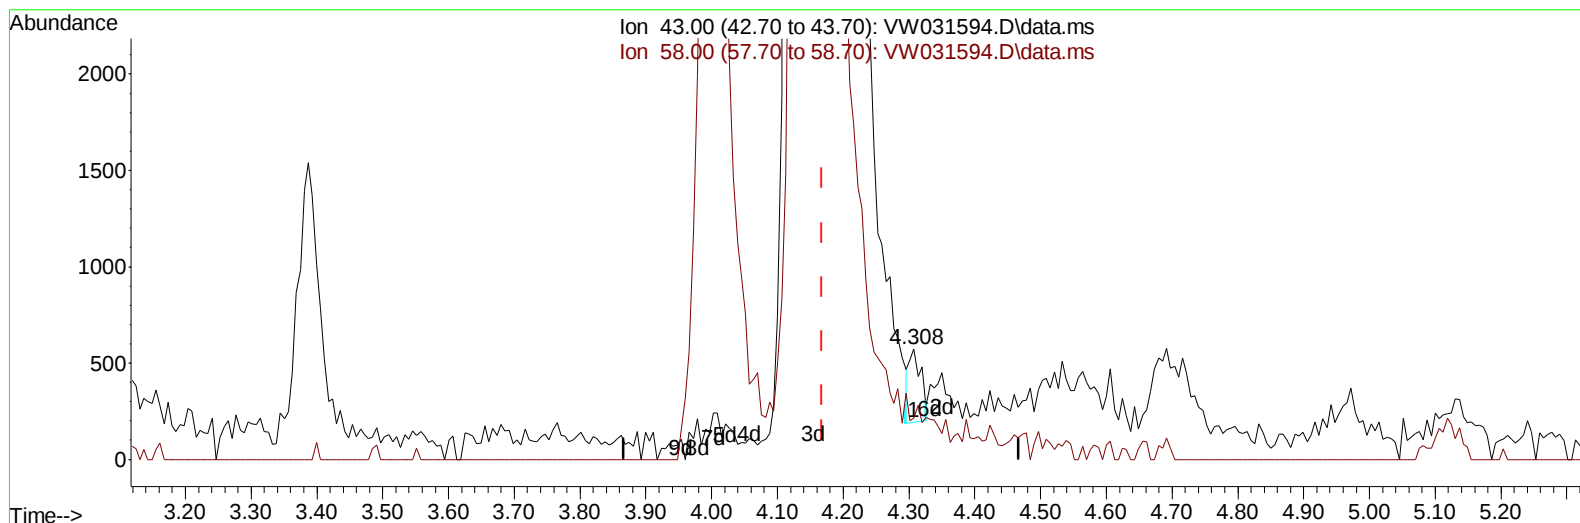

TIC: VW031594.D\data.ms

(13) Acetone (T)

4.308min (+ 0.140) 0.45 ug/L

response 479

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	9.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031594.D
Acq On : 27 Jan 2025 15:41
Operator : SY/MD
Sample : Q1190-02
Misc : 14.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:25:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

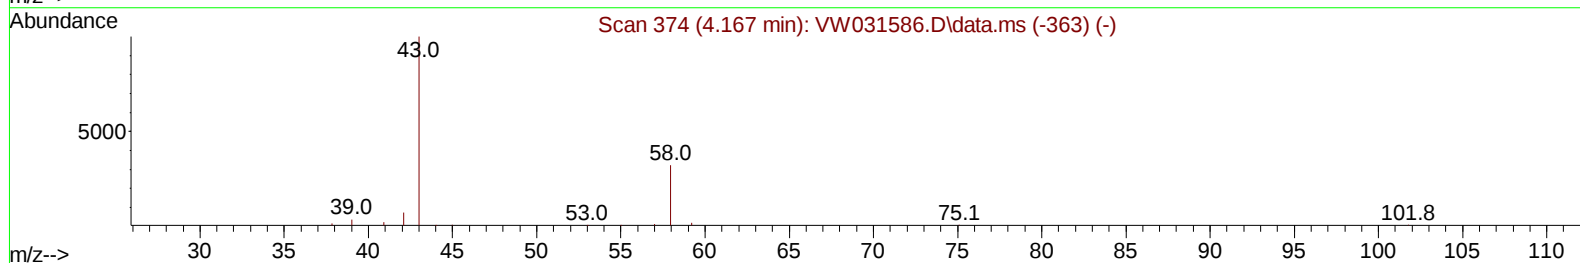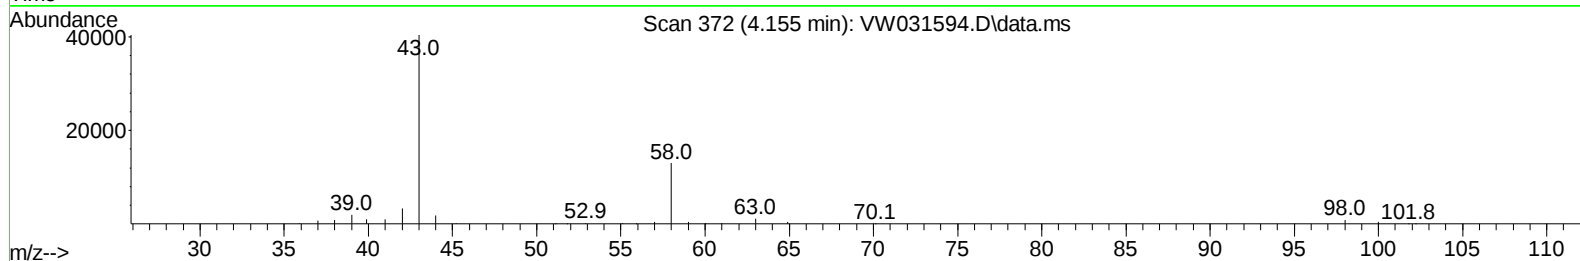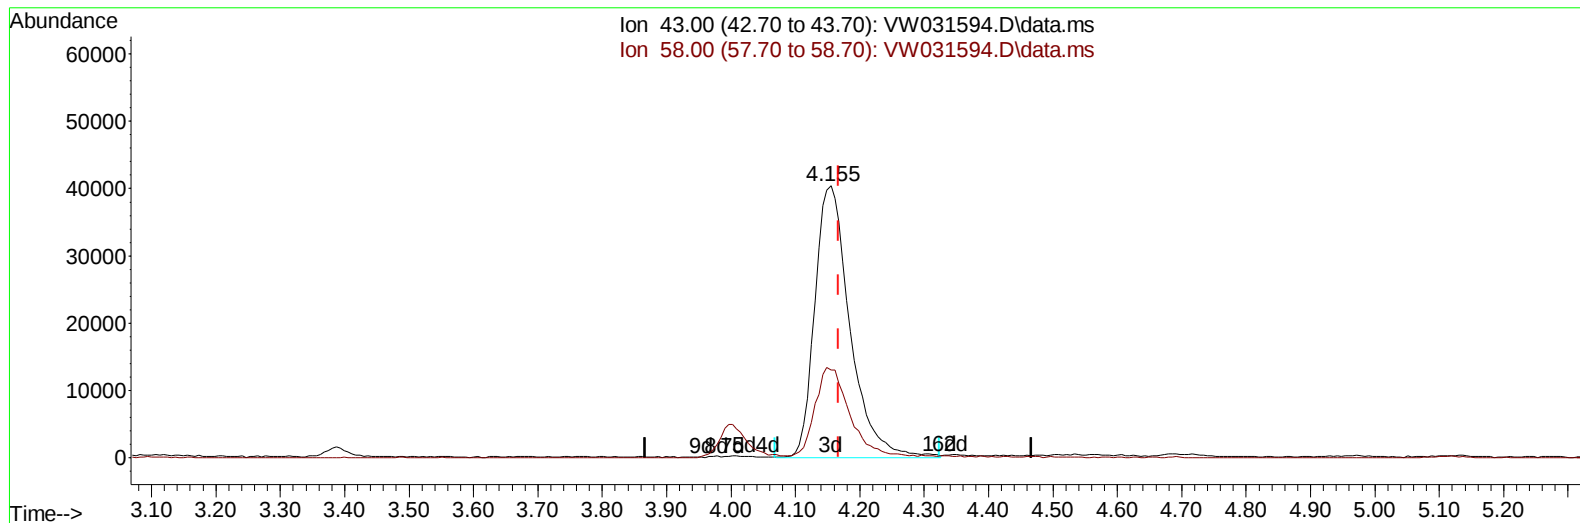

TIC: VW031594.D\data.ms

(13) Acetone (T)

4.155min (-0.012) 143.50 ug/L m

response 153081

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.03
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
 Data File : VW031594.D
 Acq On : 27 Jan 2025 15:41
 Operator : SY/MD
 Sample : Q1190-02
 Misc : 14.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44S3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/28/2025
 Supervised By :Mahesh Dadoda 01/28/2025

Quant Time: Jan 28 00:25:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 28 00:17:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	549506	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	269469	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	57128	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	195381	22.659	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	90.640%	
7) Chloroethane-d5	2.893	69	176222	28.617	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	114.480%	
11) 1,1-Dichloroethene-d2	4.021	65	85326	22.240	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	88.960%	
21) 2-Butanone-d5	7.087	46	213522	154.043	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	308.080%#	
24) Chloroform-d	7.648	84	425153	29.896	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	119.600%	
26) 1,2-Dichloroethane-d4	8.301	65	270014	38.576	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	154.320%#	
32) Benzene-d6	8.270	84	802616	47.418	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	189.680%#	
36) 1,2-Dichloropropane-d6	9.270	67	278543	55.735	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	222.960%#	
41) Toluene-d8	10.319	98	482810	31.598	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	126.400%	
43) trans-1,3-Dichloroprop...	10.575	79	77551	37.788	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	151.160%#	
47) 2-Hexanone-d5	10.922	63	134444	263.611	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	527.220%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	190792	62.427	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	249.720%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	55659	27.778	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	111.120%	
Target Compounds						
					Qvalue	
13) Acetone	4.155	43	153081m	143.497	ug/L	
22) 2-Butanone	7.191	43	15208	8.347	ug/L	81
33) Benzene	8.319	78	62014	3.363	ug/L	100
42) Toluene	10.386	91	14267	0.740	ug/L	98
46) Tetrachloroethene	10.855	164	1551	0.436	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031594.D
Acq On : 27 Jan 2025 15:41
Operator : SY/MD
Sample : Q1190-02
Misc : 14.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44S3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

Quant Time: Jan 28 00:25:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

