


Data Path : W:\HPCHEM1\MSVOA W\Data\VW012918\
Data File : VW001113.D
Acq On : 29 Jan 2018 09:45
Operator : JC/SY
Sample : BFB
Misc : 5.0G/5.0ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W012918S.M
Title : SW846 8260
Last Update : Tue Jan 30 01:11:27 2018

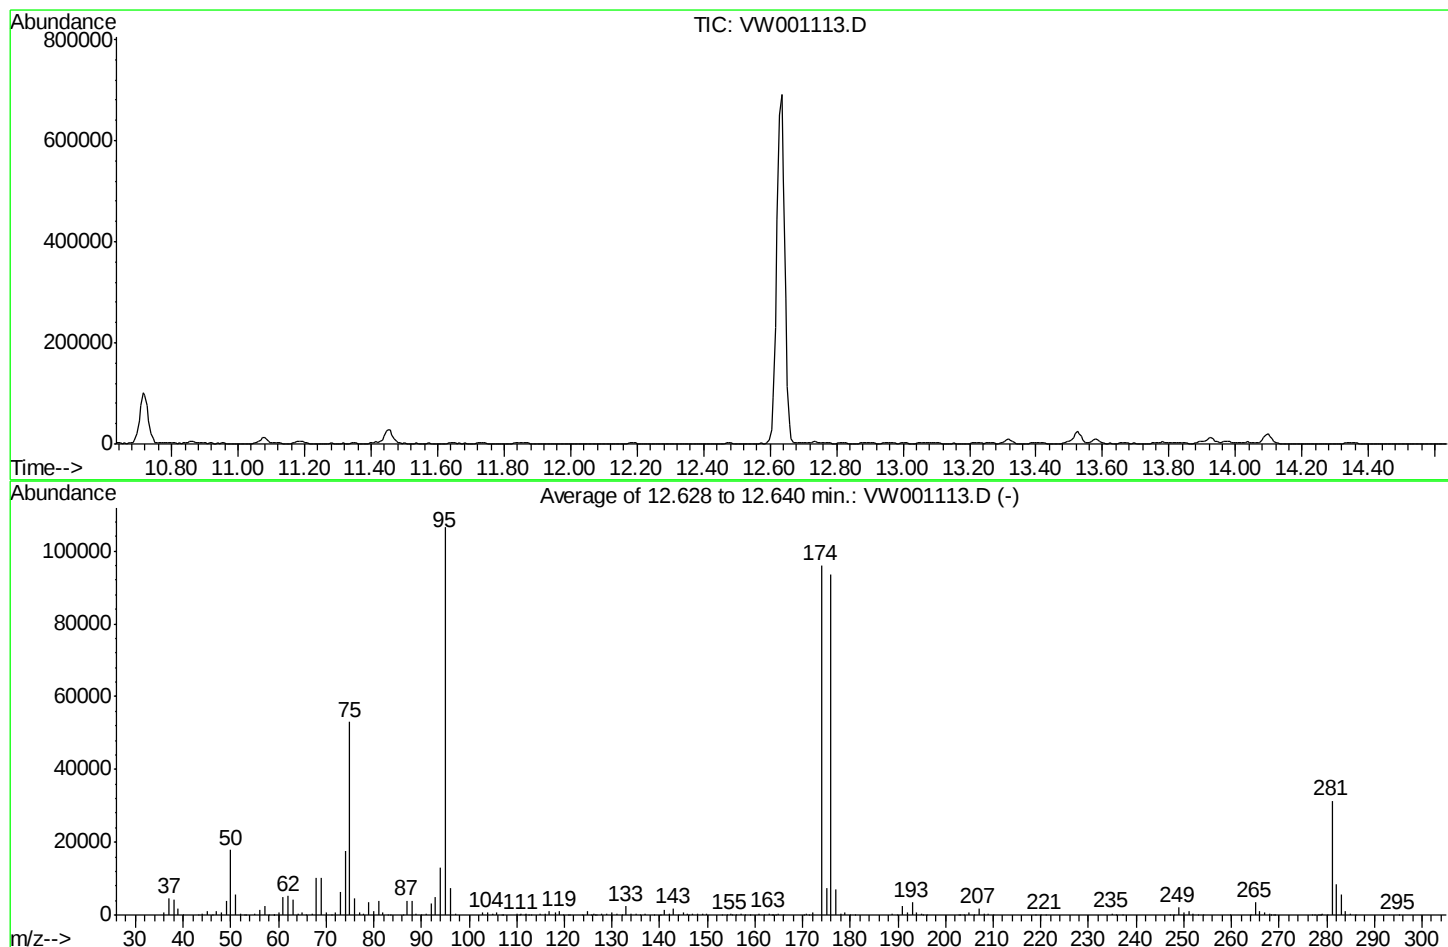

AutoFind: Scans 1811, 1812, 1813; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	17919	PASS
75	95	30	60	49.8	53069	PASS
95	95	100	100	100.0	106488	PASS
96	95	5	9	6.9	7378	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.1	95986	PASS
175	174	5	9	7.9	7549	PASS
176	174	95	101	97.3	93370	PASS
177	176	5	9	7.6	7142	PASS