


Data Path : W:\HPCHEM1\MSVOA W\Data\VW012918\
 Data File : VW001121.D
 Acq On : 29 Jan 2018 15:54
 Operator : JC/SY
 Sample : BFB
 Misc : 5.0G/5.0ML/MSVOA W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W012918S.M
 Title : SW846 8260
 Last Update : Tue Jan 30 01:11:27 2018

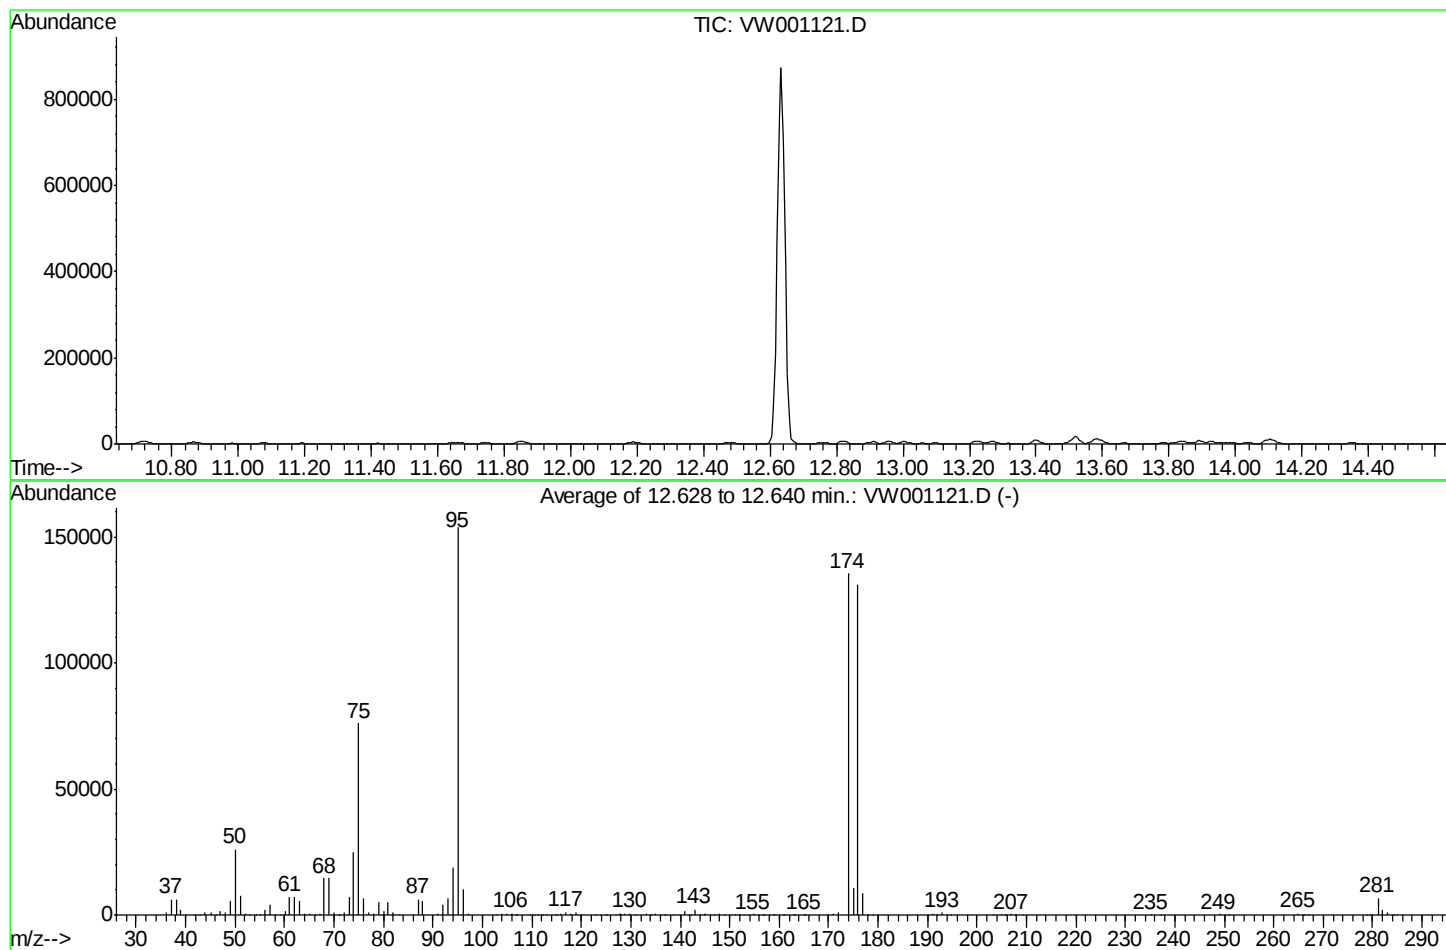

AutoFind: Scans 1811, 1812, 1813; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	26136	PASS
75	95	30	60	49.4	75944	PASS
95	95	100	100	100.0	153770	PASS
96	95	5	9	6.7	10316	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.0	135362	PASS
175	174	5	9	7.7	10446	PASS
176	174	95	101	96.7	130938	PASS
177	176	5	9	6.5	8531	PASS