




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
Data File : VW031642.D
Acq On : 29 Jan 2025 15:31
Operator : SY/MD
Sample : Q1189-04
Misc : 13.09g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q7

Manual IntegrationsAPPROVED

Quant Time: Jan 30 07:32:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 30 07:28:52 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/30/2025
Supervised By :Mahesh Dadoda 01/30/2025

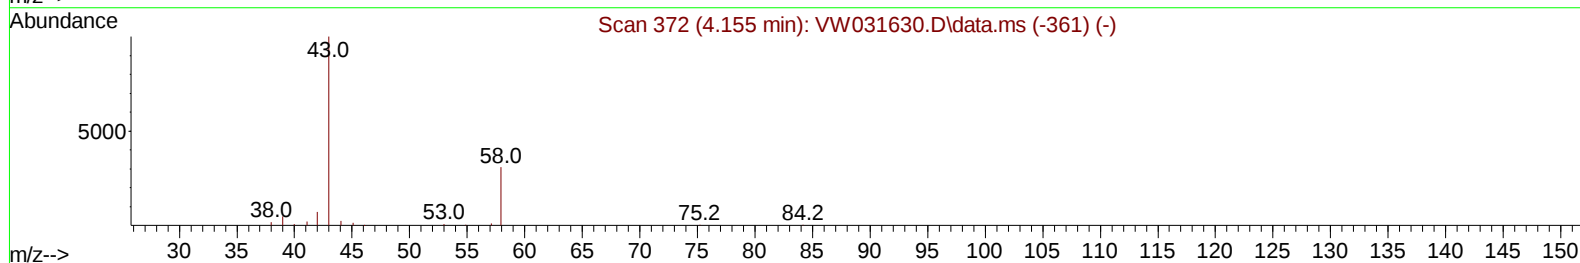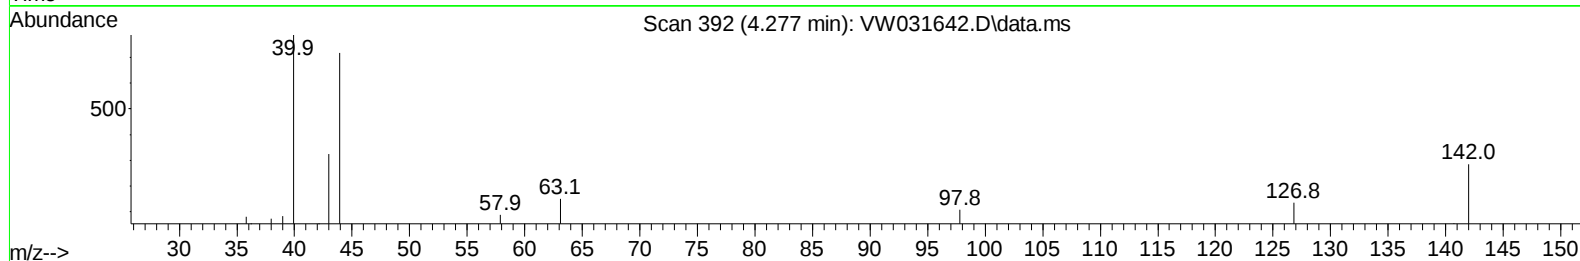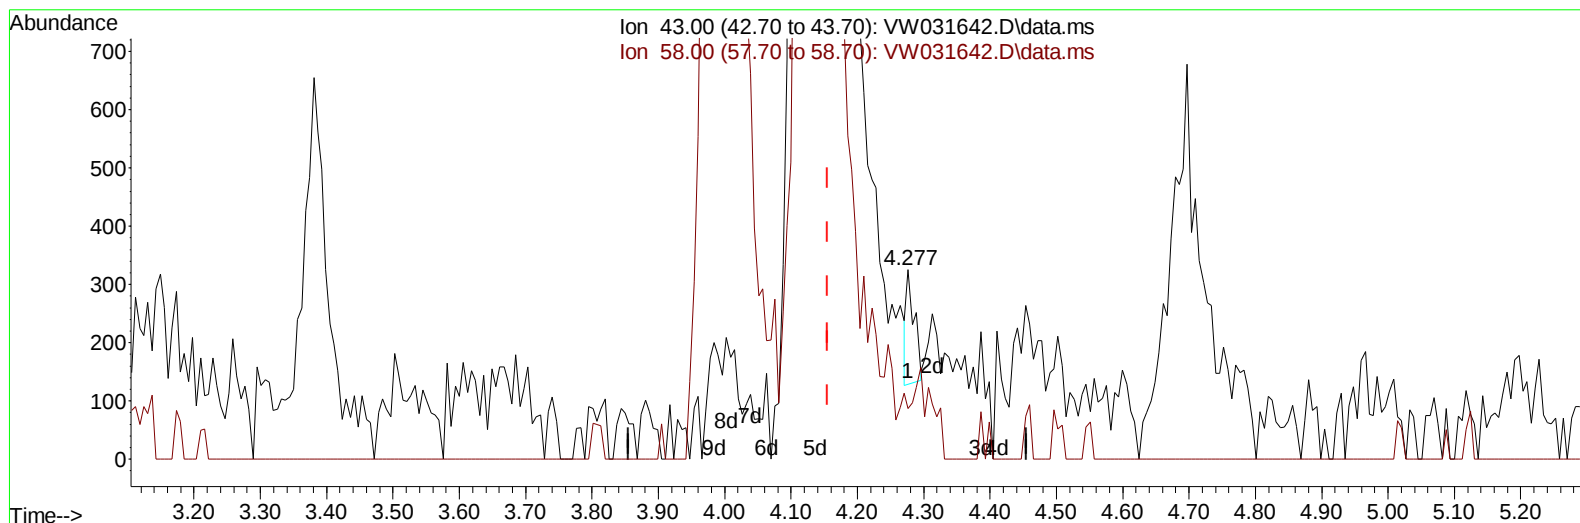

TIC: VW031642.D\data.ms

(13) Acetone (T)

4.277min (+ 0.122) 0.15 ug/L

response 159

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	23.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
Data File : VW031642.D
Acq On : 29 Jan 2025 15:31
Operator : SY/MD
Sample : Q1189-04
Misc : 13.09g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q7

Manual IntegrationsAPPROVED

Quant Time: Jan 30 07:32:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 30 07:28:52 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/30/2025
Supervised By :Mahesh Dadoda 01/30/2025

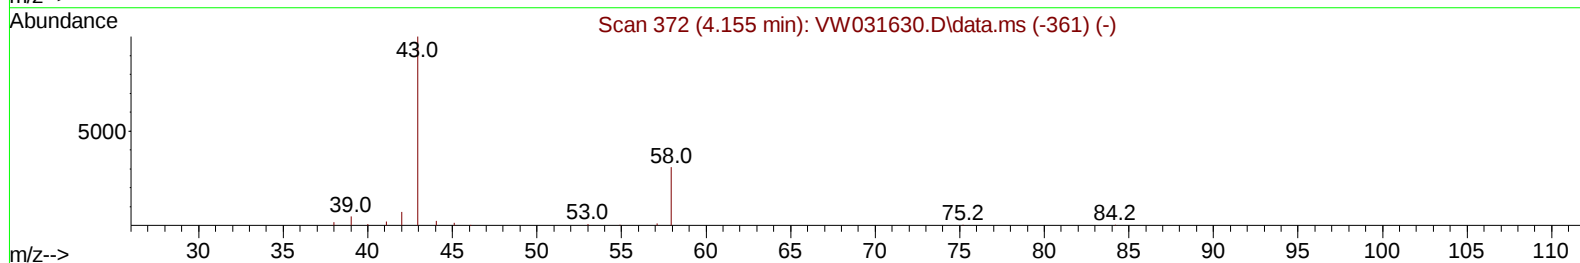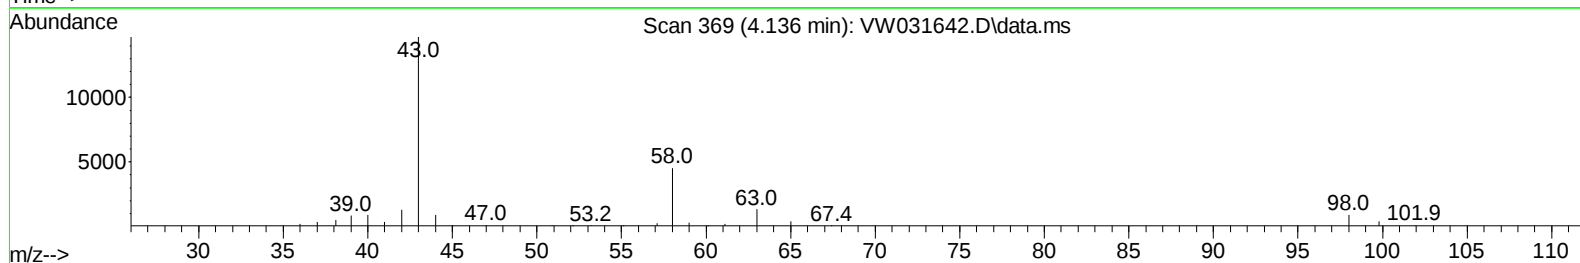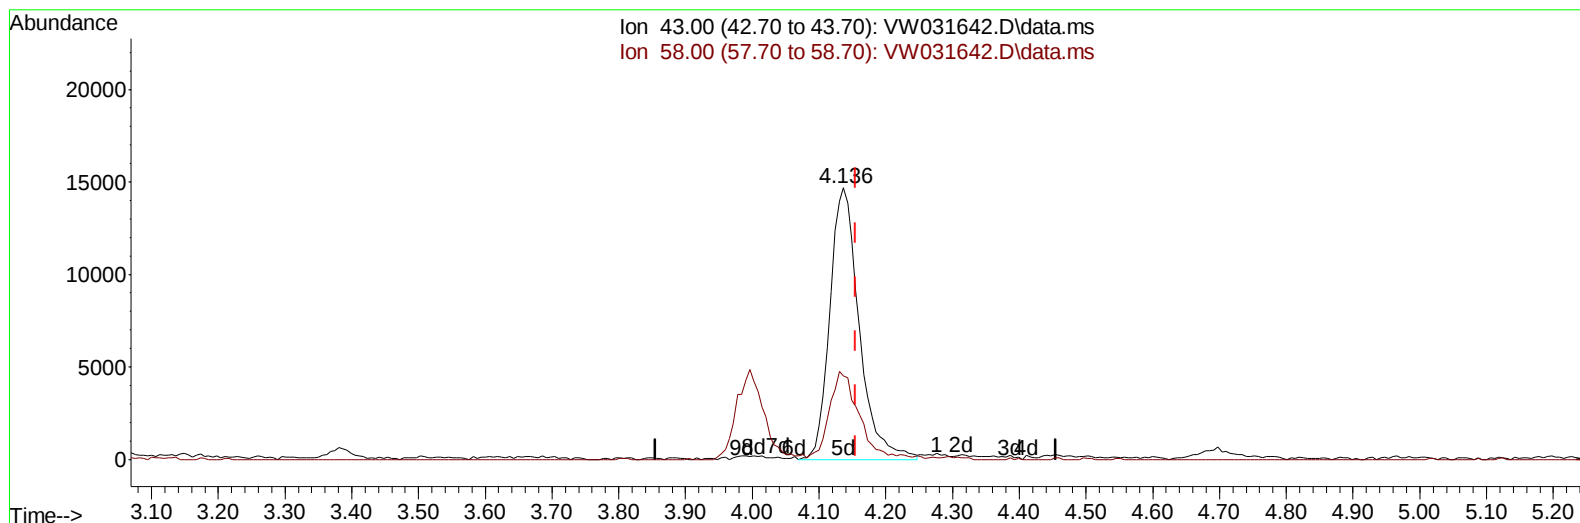

TIC: VW031642.D\data.ms

(13) Acetone (T)

4.136min (-0.018) 40.79 ug/L m

response 44632

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
 Data File : VW031642.D
 Acq On : 29 Jan 2025 15:31
 Operator : SY/MD
 Sample : Q1189-04
 Misc : 13.09g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44Q7

Manual IntegrationsAPPROVED

Quant Time: Jan 30 07:32:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jan 30 07:28:52 2025
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/30/2025
 Supervised By :Mahesh Dadoda 01/30/2025

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		563677	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		413465	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.549	152		109533	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.356	65		158050	17.869	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.480%		
7) Chloroethane-d5	2.893	69		126072	19.958	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.840%		
11) 1,1-Dichloroethene-d2	4.015	65		75939	19.296	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	77.200%		
21) 2-Butanone-d5	7.075	46		153050	107.640	ug/L	-0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	215.280%#		
24) Chloroform-d	7.642	84		345791	23.704	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	94.800%		
26) 1,2-Dichloroethane-d4	8.300	65		208700	29.066	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	116.280%		
32) Benzene-d6	8.270	84		686845	26.446	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	105.800%		
36) 1,2-Dichloropropane-d6	9.270	67		224012	29.213	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	116.840%		
41) Toluene-d8	10.318	98		537000	22.905	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	91.600%		
43) trans-1,3-Dichloroprop...	10.574	79		78685	24.988	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	99.960%		
47) 2-Hexanone-d5	10.922	63		106005	135.462	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	270.920%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		213363	45.499	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	182.000%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		100788	26.235	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	104.920%		
Target Compounds							
13) Acetone	4.136	43		44632m	40.786	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
Data File : VW031642.D
Acq On : 29 Jan 2025 15:31
Operator : SY/MD
Sample : Q1189-04
Misc : 13.09g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/30/2025
Supervised By :Mahesh Dadoda 01/30/2025

Quant Time: Jan 30 07:32:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 30 07:28:52 2025
Response via : Initial Calibration

