




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
Data File : VW031651.D
Acq On : 29 Jan 2025 19:10
Operator : SY/MD
Sample : Q1189-17
Misc : 21.37g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44R8

Manual IntegrationsAPPROVED

Quant Time: Jan 30 07:34:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 30 07:28:52 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/30/2025
Supervised By :Mahesh Dadoda 01/30/2025

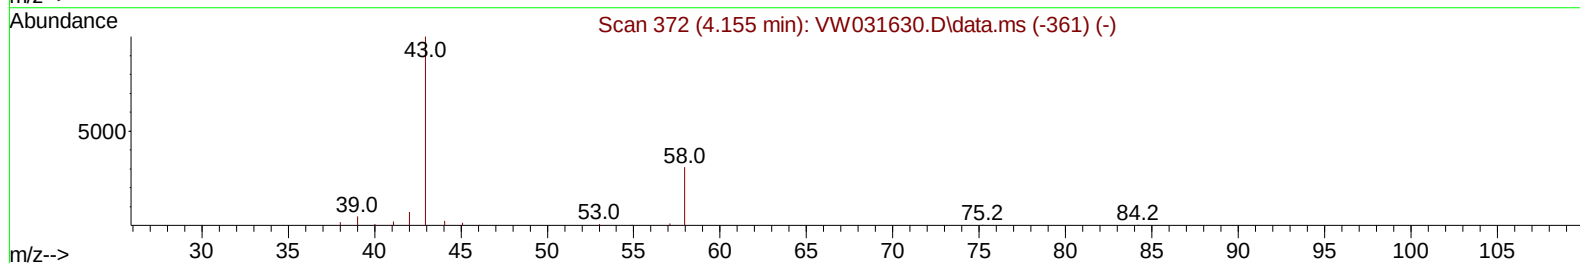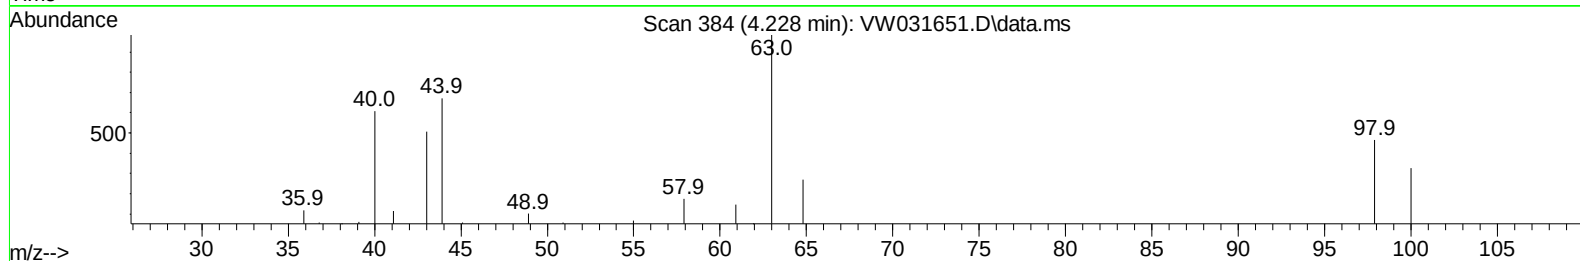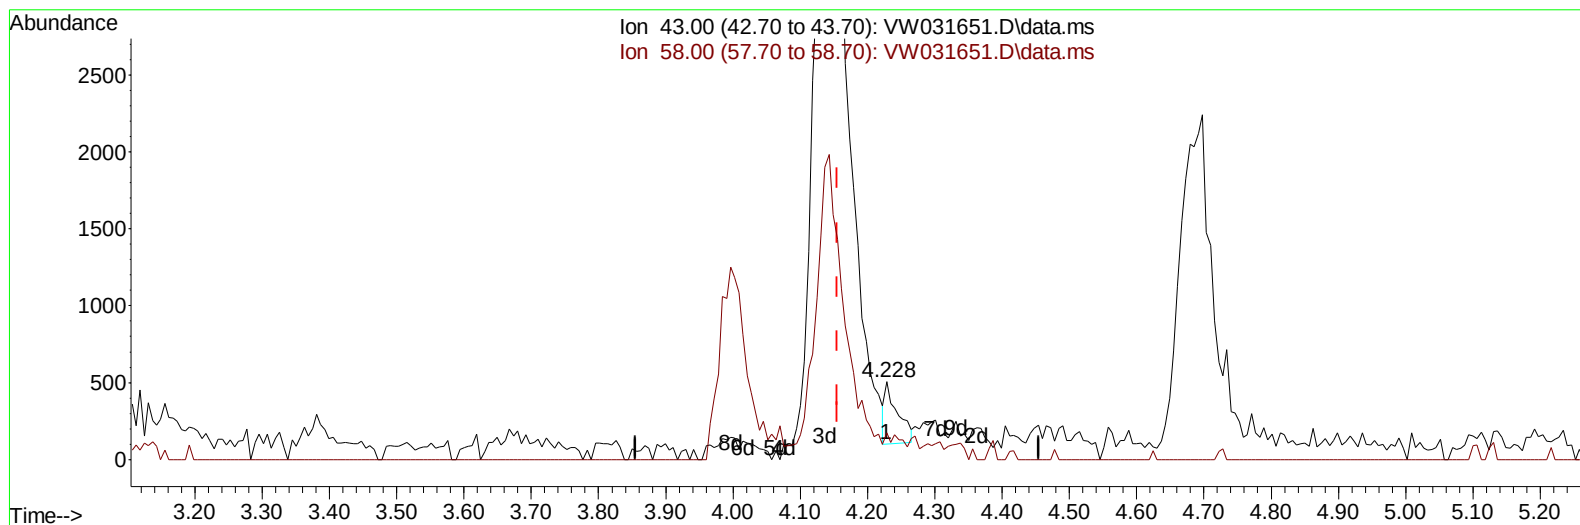

TIC: VW031651.D\data.ms

(13) Acetone (T)

4.228min (+ 0.073) 0.32 ug/L

response 541

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	19.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
Data File : VW031651.D
Acq On : 29 Jan 2025 19:10
Operator : SY/MD
Sample : Q1189-17
Misc : 21.37g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44R8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/30/2025
Supervised By :Mahesh Dadoda 01/30/2025

Quant Time: Jan 30 07:34:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 30 07:28:52 2025
Response via : Initial Calibration

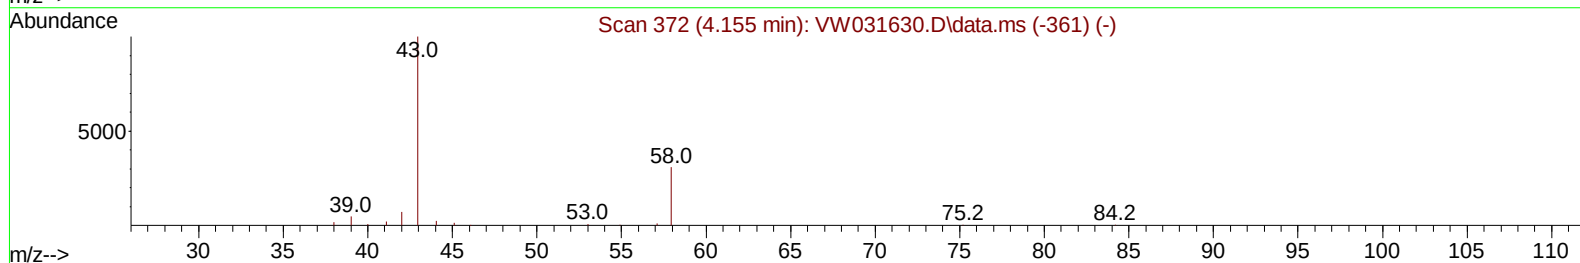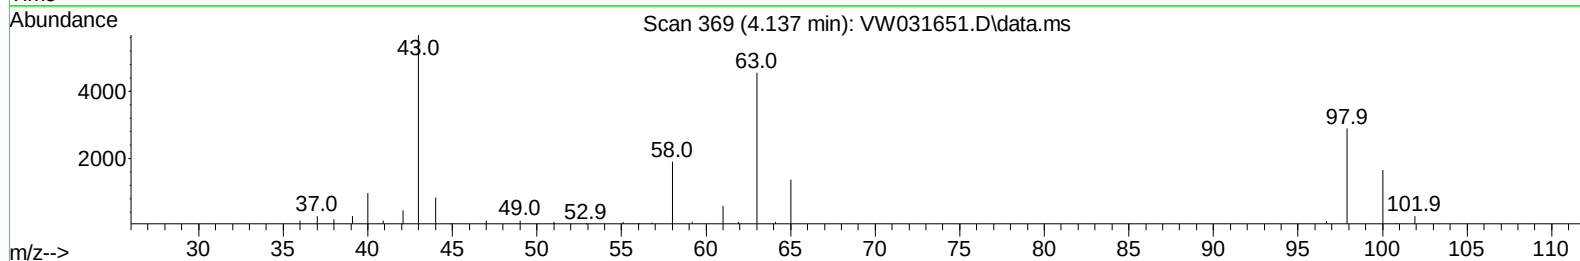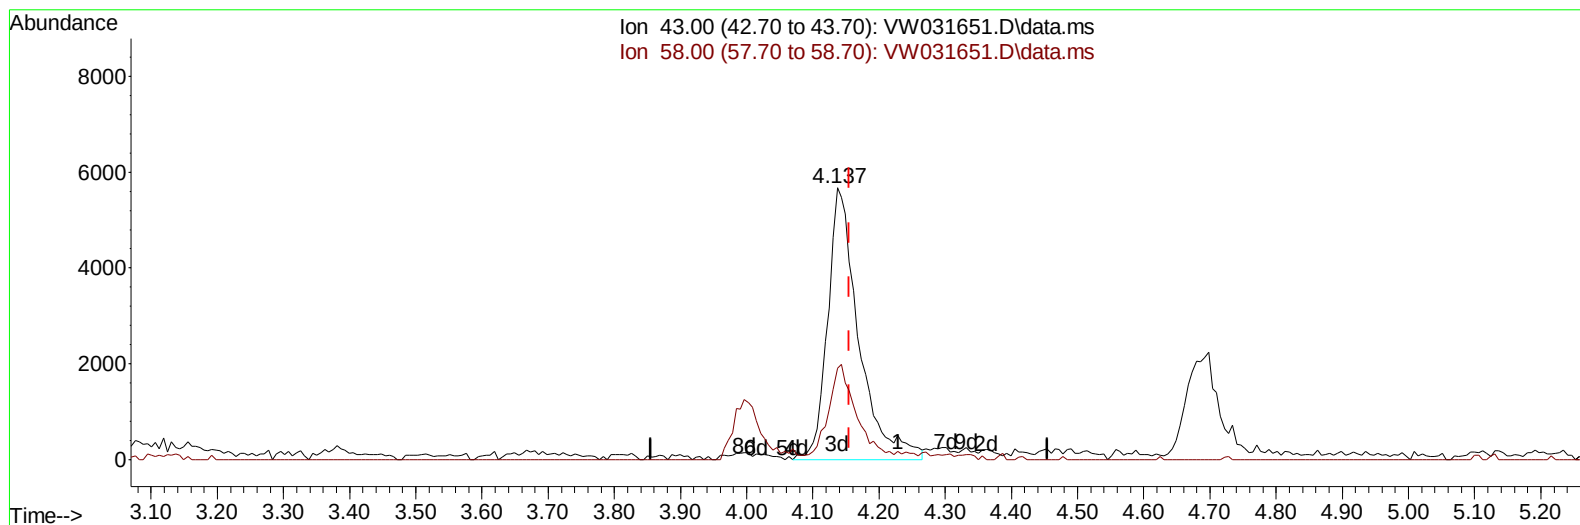

TIC: VW031651.D\data.ms

(13) Acetone (T)

4.137min (-0.018) 10.80 ug/L m

response 18485

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.56
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
 Data File : VW031651.D
 Acq On : 29 Jan 2025 19:10
 Operator : SY/MD
 Sample : Q1189-17
 Misc : 21.37g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44R8

Manual IntegrationsAPPROVED

Quant Time: Jan 30 07:34:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jan 30 07:28:52 2025
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/30/2025
 Supervised By :Mahesh Dadoda 01/30/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	881816	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	776012	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	303467	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	223152	16.127	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	64.520%	
7) Chloroethane-d5	2.893	69	173411	17.548	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.200%	
11) 1,1-Dichloroethene-d2	4.015	65	107074	17.392	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.560%	
21) 2-Butanone-d5	7.081	46	210233	94.514	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	189.020%#	
24) Chloroform-d	7.642	84	499010	21.866	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	87.480%	
26) 1,2-Dichloroethane-d4	8.301	65	307349	27.362	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	109.440%	
32) Benzene-d6	8.270	84	1005023	20.618	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.480%	
36) 1,2-Dichloropropane-d6	9.270	67	331723	23.049	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.200%	
41) Toluene-d8	10.319	98	867275	19.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.840%	
43) trans-1,3-Dichloroprop...	10.575	79	134941	22.832	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.320%	
47) 2-Hexanone-d5	10.922	63	150512	102.479	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	204.960%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	326195	37.062	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	148.240%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	238738	22.430	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.720%	
Target Compounds					Qvalue	
13) Acetone	4.137	43	18485m	10.798	ug/L	
15) Methyl Acetate	4.698	43	6653	1.483	ug/L #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012925\
Data File : VW031651.D
Acq On : 29 Jan 2025 19:10
Operator : SY/MD
Sample : Q1189-17
Misc : 21.37g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44R8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/30/2025
Supervised By :Mahesh Dadoda 01/30/2025

Quant Time: Jan 30 07:34:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 30 07:28:52 2025
Response via : Initial Calibration

