

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013023\
 Data File : VW025249.D
 Acq On : 30 Jan 2023 14:28
 Operator : SY/MD
 Sample : VW0130SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 31 01:38:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM013023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 31 01:26:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	406971	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	368747	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	174352	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	104900	23.084	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.320%
7) Chloroethane-d5	2.879	69	66881	22.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	4.013	63	180442	16.913	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.640%
21) 2-Butanone-d5	7.080	46	60310	48.615	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.220%
24) Chloroform-d	7.647	84	250974	23.244	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.960%
26) 1,2-Dichloroethane-d4	8.305	65	137735	23.816	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.280%
32) Benzene-d6	8.275	84	520878	23.821	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.280%
36) 1,2-Dichloropropane-d6	9.274	67	148436	23.454	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.800%
41) Toluene-d8	10.323	98	477990	23.687	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.760%
43) trans-1,3-Dichloroprop...	10.579	79	64869	23.276	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.120%
47) 2-Hexanone-d5	10.921	63	49939	49.439	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.880%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	113683	23.318	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	148412	23.821	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.280%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.274	63	17936	3.073	ug/L	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013023\
Data File : VW025249.D
Acq On : 30 Jan 2023 14:28
Operator : SY/MD
Sample : VW0130SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jan 31 01:38:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM013023SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 31 01:26:27 2023
Response via : Initial Calibration

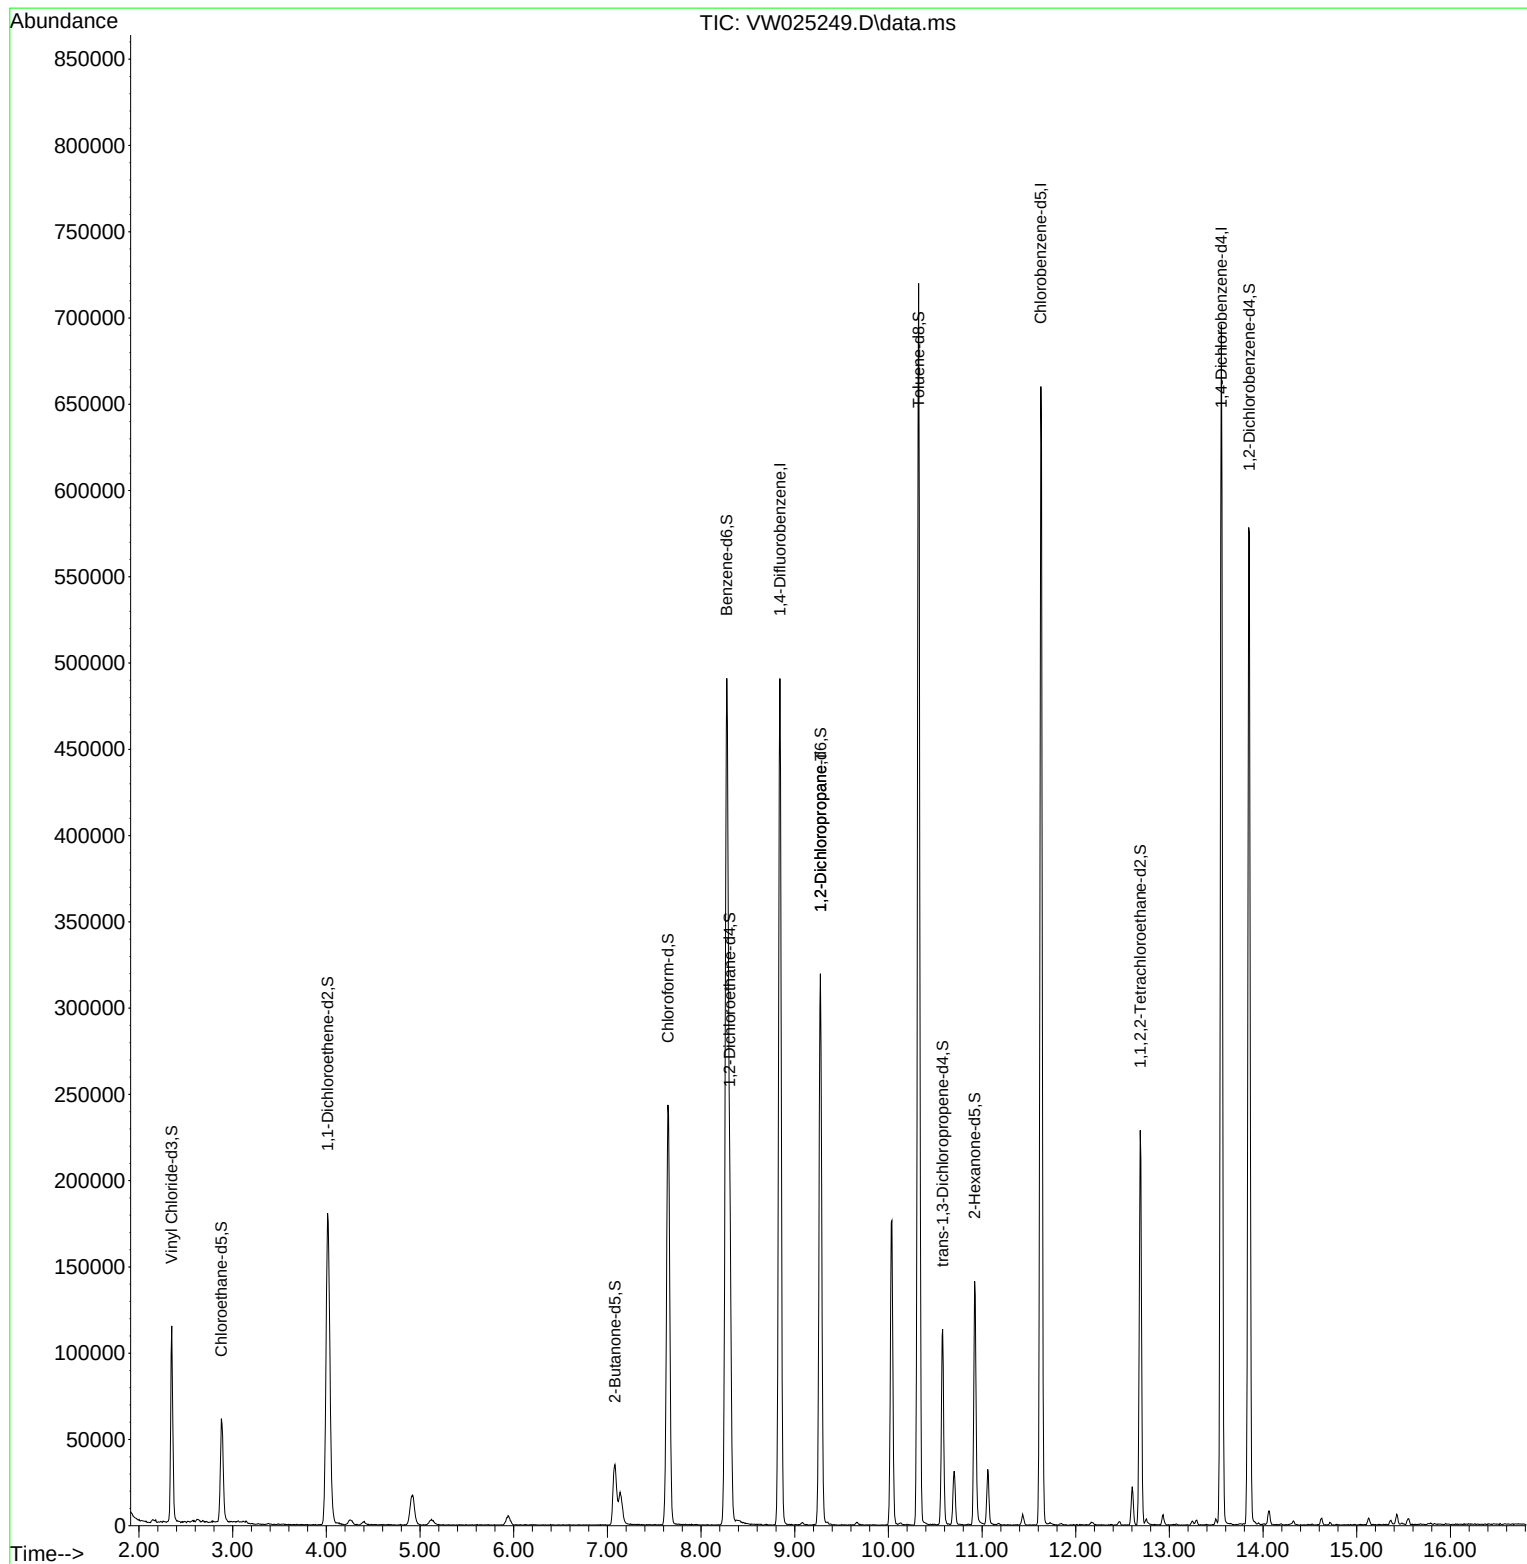

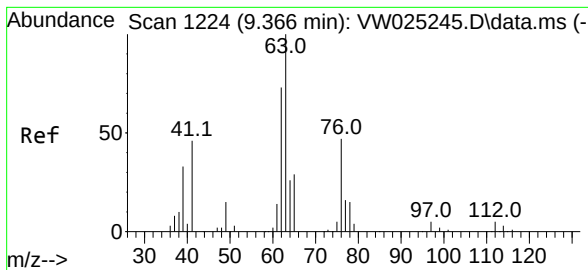

#37
 1,2-Dichloropropane
 Concen: 3.073 ug/L
 RT: 9.274 min Scan# 11
 Delta R.T. -0.091 min
 Lab File: VW025249.D
 Acq: 30 Jan 2023 14:28

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 63 Resp: 17936
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.8#

