


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013024\
Data File : VW027860.D
Acq On : 30 Jan 2024 10:36
Operator : SY/MD
Sample : BFB428
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB428

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Title : SFAM01.0
Last Update : Tue Jan 30 22:00:20 2024

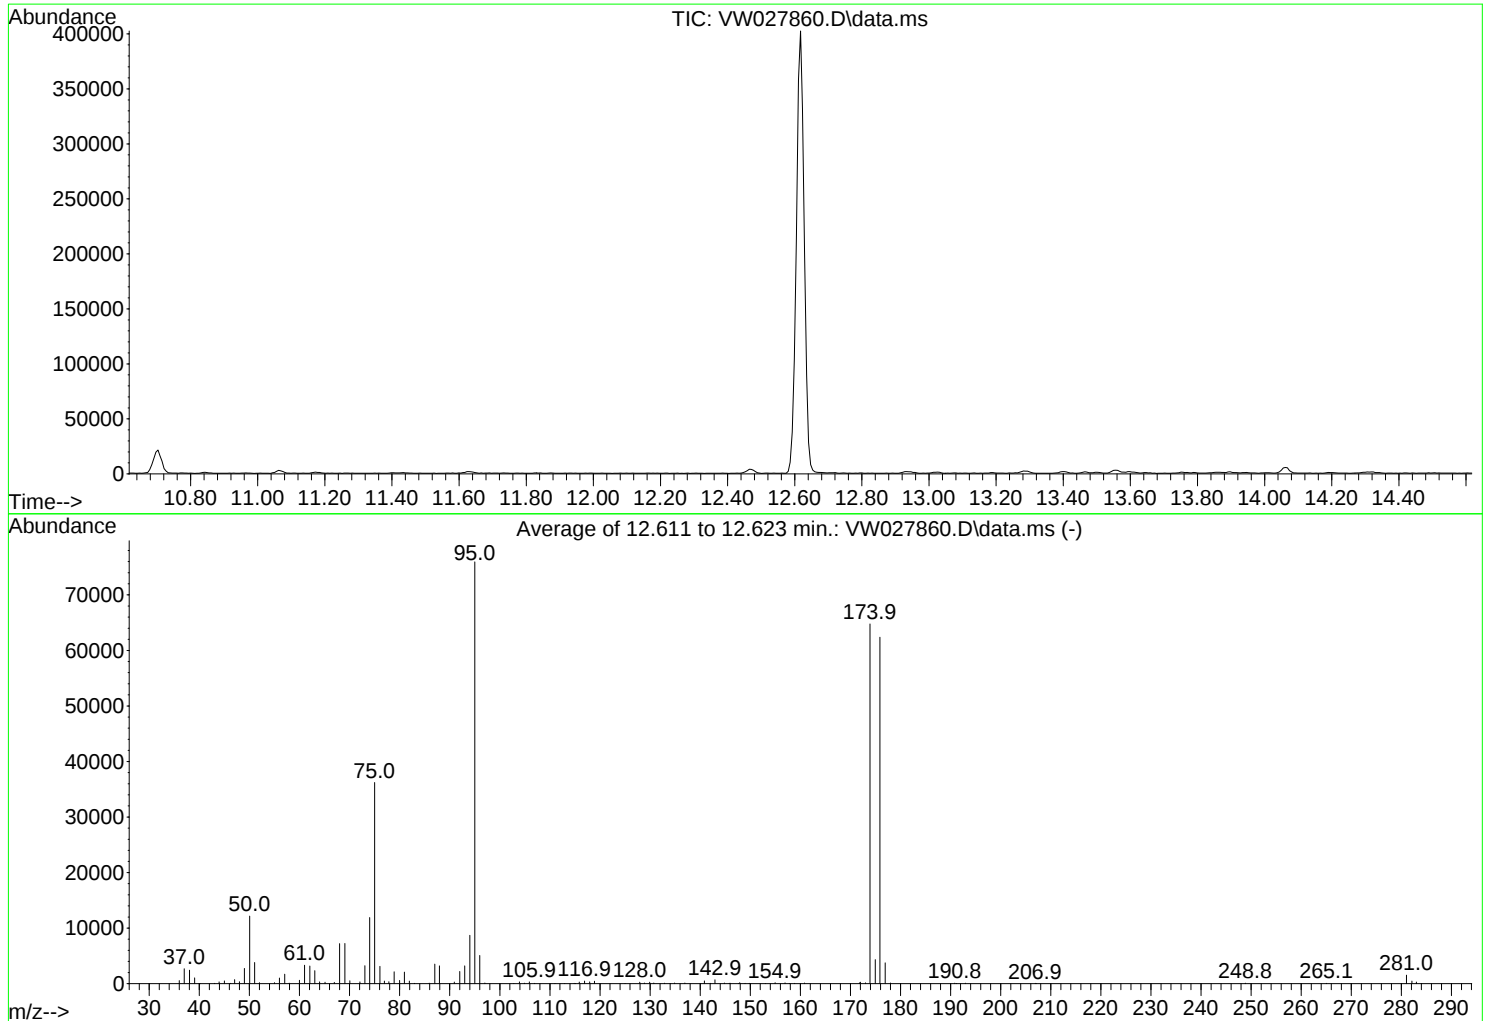

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	12154	PASS
75	95	30	80	47.7	36213	PASS
95	95	100	100	100.0	75955	PASS
96	95	5	9	6.7	5068	PASS
173	174	0.00	2	0.2	136	PASS
174	95	50	120	85.3	64773	PASS
175	174	5	9	6.7	4330	PASS
176	174	95	101	96.3	62381	PASS
177	176	5	9	6.0	3745	PASS

Scan 1752 (12.568 min): VW027860.D\data.ms
BFB428

m/z	Abundance
40.00	503.0
43.90	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB428

m/z	Abundance
36.00	455.0
37.00	2683.0
38.00	2502.0
39.10	972.0
40.00	556.0
43.00	54.0
44.00	367.0
45.00	544.0
46.20	90.0
47.10	842.0
48.10	372.0
49.00	2638.0
50.10	12689.0
51.00	3805.0
52.10	160.0
55.00	197.0
56.00	1046.0
57.10	1985.0
58.00	121.0
60.00	570.0
61.00	3454.0
62.00	3360.0
63.10	2519.0
64.00	313.0
65.20	253.0
67.00	204.0
68.00	7296.0
69.00	7437.0
70.00	508.0
72.00	292.0
73.00	3446.0
74.00	12293.0
75.00	37656.0
76.00	3442.0
77.00	519.0
78.00	427.0
78.90	2076.0
80.00	556.0
81.00	1914.0
81.90	476.0
82.90	118.0
85.90	106.0
87.00	3503.0
87.90	3340.0
90.90	248.0
92.00	2089.0
93.00	3209.0
94.00	8262.0
95.00	74920.0
96.00	5188.0
97.10	130.0
103.90	328.0
105.00	107.0
105.90	313.0
106.90	66.0
113.00	72.0
115.10	90.0
115.80	298.0
116.90	483.0
118.00	243.0
118.90	555.0
125.00	91.0
128.00	241.0
128.90	154.0
129.80	200.0
130.80	105.0
132.90	246.0
134.00	52.0
134.90	118.0
136.90	90.0
140.90	386.0
142.90	644.0
144.90	132.0
145.80	107.0
147.70	127.0
148.90	60.0
155.00	154.0
156.90	137.0
158.90	62.0
160.90	78.0
171.80	406.0
173.00	407.0
173.90	57960.0
175.00	4301.0
175.90	58808.0
176.90	3620.0
178.00	101.0
190.90	174.0
193.00	112.0
206.90	152.0
248.80	192.0
265.00	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB428

281.00	2499.0
282.10	742.0
283.00	546.0
284.00	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB428

m/z	Abundance
36.00	659.0
37.00	2942.0
38.10	2666.0
39.00	1217.0
39.90	489.0
43.10	62.0
44.00	590.0
45.00	558.0
46.30	67.0
47.10	699.0
47.90	419.0
49.00	3125.0
50.00	13320.0
51.10	4133.0
52.00	192.0
55.00	180.0
56.00	1045.0
57.00	1714.0
58.00	69.0
60.00	590.0
61.00	3608.0
62.10	3404.0
63.00	2459.0
64.00	376.0
65.00	357.0
66.90	267.0
68.00	8007.0
69.00	7952.0
70.00	582.0
72.00	360.0
73.00	3455.0
74.00	13073.0
75.00	40328.0
76.00	3399.0
76.90	383.0
77.80	343.0
78.90	2475.0
80.00	653.0
80.90	2252.0
82.00	484.0
85.90	121.0
87.00	3720.0
88.00	3269.0
90.90	376.0
92.00	2584.0
93.00	3409.0
94.00	9426.0
95.00	85776.0
96.00	5569.0
96.90	173.0
102.80	89.0
103.90	434.0
104.90	113.0
105.90	392.0
106.90	55.0
111.00	95.0
112.90	67.0
114.80	95.0
115.90	350.0
116.90	532.0
118.00	429.0
118.90	451.0
127.80	324.0
128.90	106.0
129.90	368.0
130.70	165.0
132.80	60.0
134.90	118.0
137.00	142.0
140.80	599.0
142.00	162.0
142.90	763.0
144.80	101.0
146.00	137.0
147.90	259.0
149.00	69.0
149.80	86.0
154.90	215.0
157.00	163.0
157.80	59.0
158.90	64.0
160.80	147.0
172.00	382.0
173.90	71104.0
175.00	4499.0
175.90	69472.0
177.00	3898.0
178.00	106.0
190.80	80.0
191.20	50.0
192.90	89.0
207.10	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB428

248.90	72.0
265.10	64.0
281.00	1391.0
282.10	466.0
283.00	242.0
284.10	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB428

m/z	Abundance
36.00	501.0
37.00	2382.0
38.00	2121.0
39.10	903.0
40.00	492.0
43.00	66.0
44.00	406.0
45.00	401.0
47.00	615.0
48.00	219.0
49.00	2416.0
50.00	10453.0
51.00	3464.0
51.90	130.0
55.00	142.0
56.00	954.0
57.00	1418.0
57.90	80.0
60.00	673.0
61.00	2879.0
62.00	2729.0
63.00	2010.0
64.00	229.0
65.10	165.0
67.00	211.0
68.00	6335.0
69.10	6289.0
70.10	509.0
72.10	327.0
73.10	2768.0
74.00	10332.0
75.00	30656.0
76.10	2495.0
77.00	469.0
77.80	302.0
78.90	1848.0
80.00	561.0
80.90	2092.0
81.90	394.0
83.00	72.0
87.00	3369.0
87.90	3012.0
90.90	204.0
92.00	1914.0
93.00	2957.0
94.00	8402.0
95.00	67168.0
96.00	4448.0
97.00	86.0
103.90	197.0
104.80	71.0
105.90	226.0
107.00	82.0
114.90	102.0
115.90	219.0
116.90	360.0
117.90	255.0
119.00	332.0
128.00	261.0
128.80	118.0
130.00	187.0
130.80	83.0
134.90	154.0
137.00	152.0
140.90	525.0
142.10	54.0
143.00	670.0
144.90	109.0
145.90	92.0
147.90	239.0
149.00	55.0
149.80	76.0
153.00	58.0
154.90	139.0
157.00	123.0
158.80	62.0
160.80	99.0
172.00	411.0
173.90	65256.0
174.90	4189.0
175.90	58864.0
176.90	3717.0
178.00	133.0
192.90	53.0
281.10	663.0
281.90	140.0
283.00	105.0

Instrument :
MSVOA_W
ClientSampleId :
BFB428