

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
 Data File : VW031656.D
 Acq On : 30 Jan 2025 14:44
 Operator : SY/MD
 Sample : VW0130SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 31 07:34:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 31 07:33:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	585506	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	512611	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	238794	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	168920	18.386	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.560%
7) Chloroethane-d5	2.893	69	130366	19.869	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.480%
11) 1,1-Dichloroethene-d2	4.015	65	83072	20.322	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.280%
21) 2-Butanone-d5	7.087	46	81496	55.179	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.360%
24) Chloroform-d	7.648	84	346267	22.851	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	8.301	65	185470	24.868	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.480%
32) Benzene-d6	8.270	84	725366	22.527	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.120%
36) 1,2-Dichloropropane-d6	9.270	67	221037	23.250	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.000%
41) Toluene-d8	10.319	98	644816	22.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.720%
43) trans-1,3-Dichloroprop...	10.575	79	81347	20.837	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.360%
47) 2-Hexanone-d5	10.922	63	53544	55.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.380%
56) 1,1,2,2-Tetrachloroeth...	12.684	84	157293	27.055	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	199892	23.866	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.480%
Target Compounds						
16) Methylene chloride	4.917	84	2870	0.360	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031656.D
Acq On : 30 Jan 2025 14:44
Operator : SY/MD
Sample : VW0130SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jan 31 07:34:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

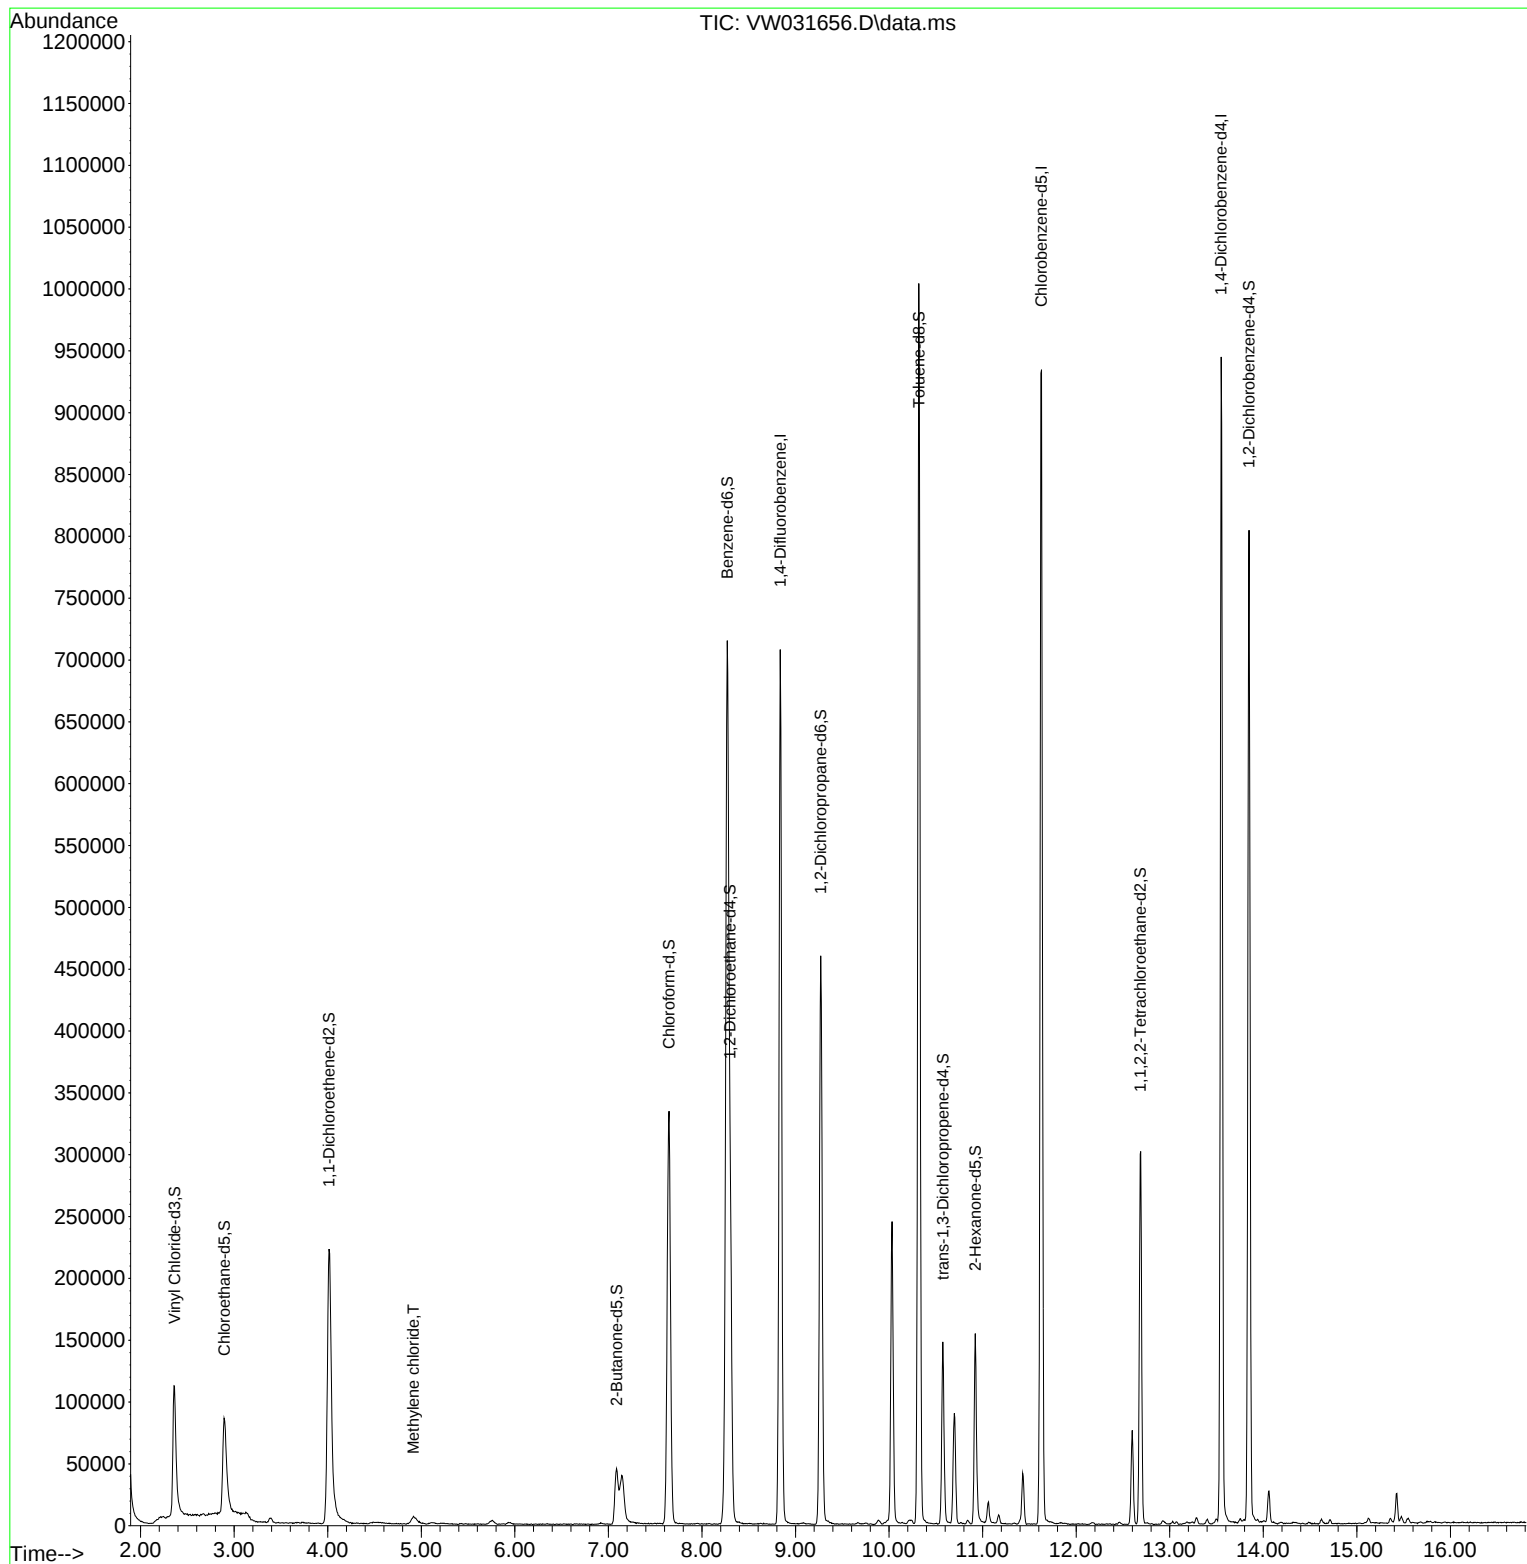

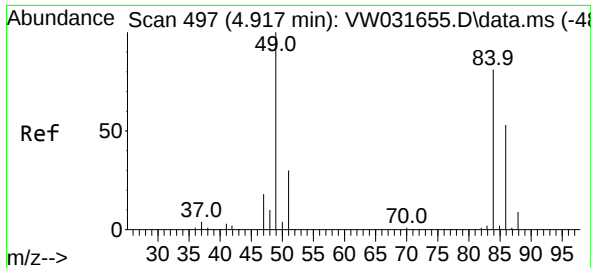

#16
Methylene chloride
Concen: 0.360 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW031656.D
Acq: 30 Jan 2025 14:44

Instrument :
MSVOA_W
ClientSampleId :

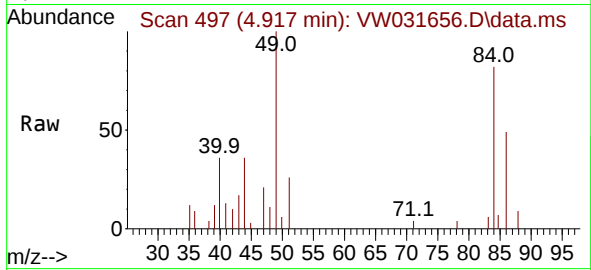

Tgt Ion: 84 Resp: 2870
Ion Ratio Lower Upper
84 100
86 54.8 47.0 87.2
49 112.8 89.8 166.8

