




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031657.D
Acq On : 30 Jan 2025 15:21
Operator : SY/MD
Sample : Q1189-08RE
Misc : 9.50g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44R1RE

Manual IntegrationsAPPROVED

Quant Time: Jan 31 07:35:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/31/2025
Supervised By :Mahesh Dadoda 01/31/2025

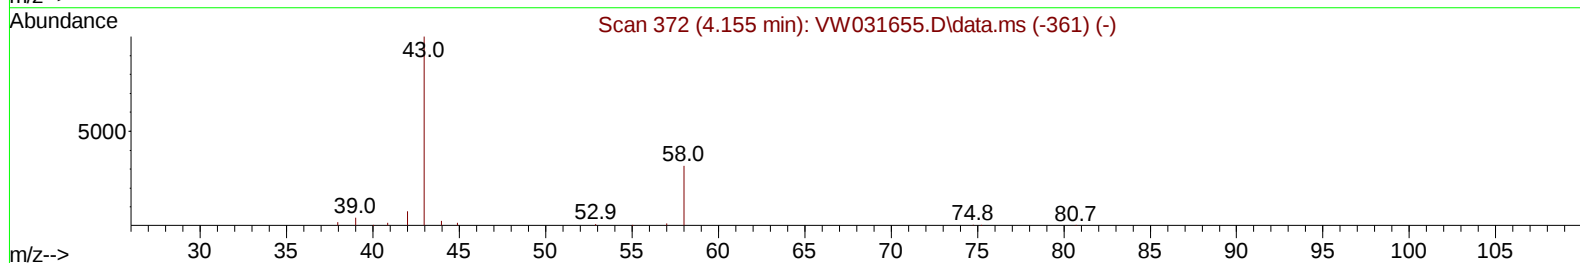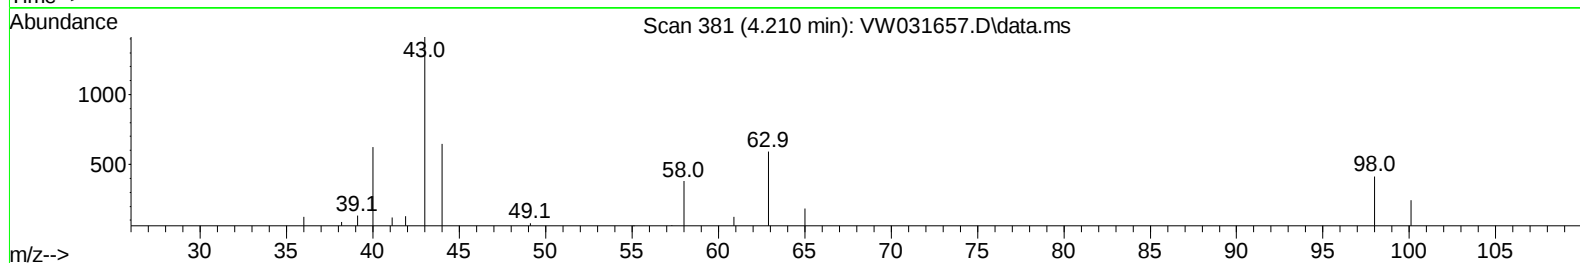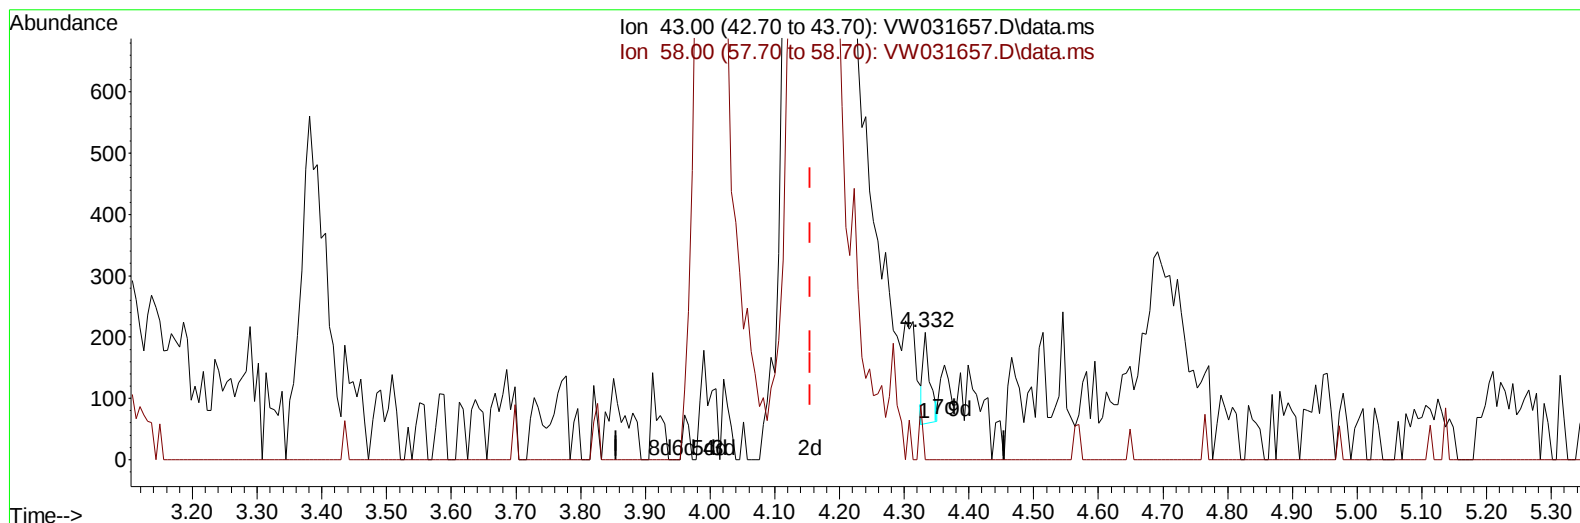

TIC: VW031657.D\data.ms

(13) Acetone (T)

4.332min (+ 0.177) 0.06 ug/L

response 106

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	22.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031657.D
Acq On : 30 Jan 2025 15:21
Operator : SY/MD
Sample : Q1189-08RE
Misc : 9.50g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44R1RE

Manual IntegrationsAPPROVED

Quant Time: Jan 31 07:35:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/31/2025
Supervised By :Mahesh Dadoda 01/31/2025

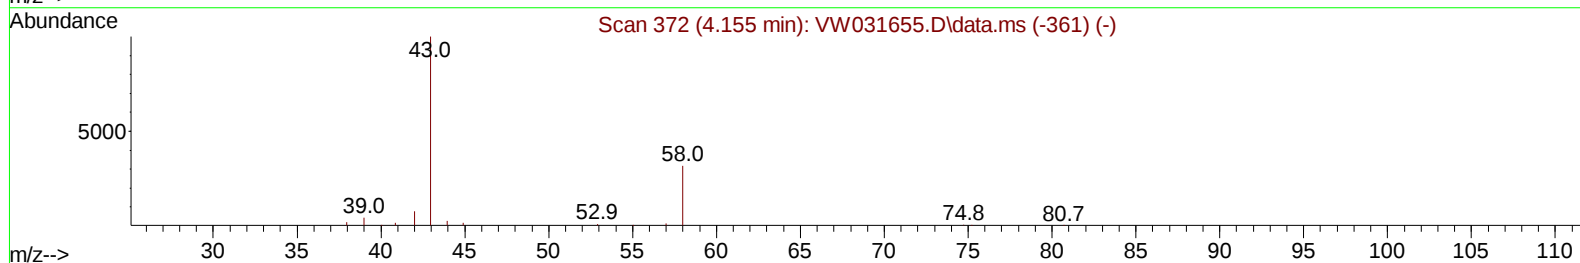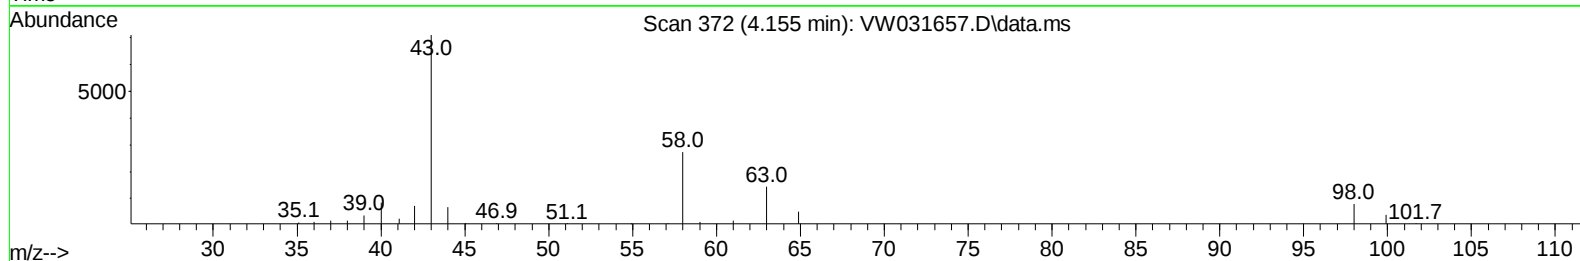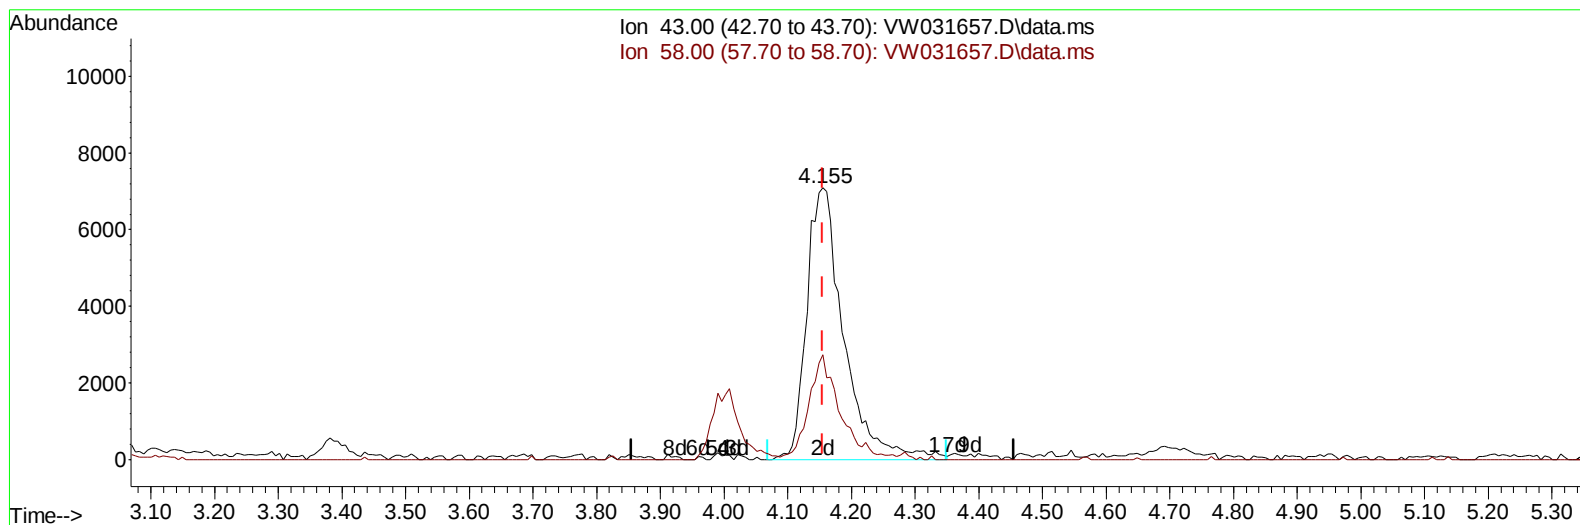

TIC: VW031657.D\data.ms

(13) Acetone (T)

4.155min (+ 0.000) 15.81 ug/L m

response 28698

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
 Data File : VW031657.D
 Acq On : 30 Jan 2025 15:21
 Operator : SY/MD
 Sample : Q1189-08RE
 Misc : 9.50g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44R1RE

Manual IntegrationsAPPROVED

Quant Time: Jan 31 07:35:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 31 07:33:50 2025
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/31/2025
 Supervised By :Mahesh Dadoda 01/31/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	934797	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.623	117	833338	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	382761	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	174339	11.885	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.560%	
7) Chloroethane-d5	2.893	69	140934	13.453	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	53.800%	
11) 1,1-Dichloroethene-d2	4.015	65	91252	13.982	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.920%	
21) 2-Butanone-d5	7.082	46	131103	55.599	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	111.200%	
24) Chloroform-d	7.642	84	418254	17.288	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	69.160%	
26) 1,2-Dichloroethane-d4	8.301	65	242046	20.327	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	81.320%	
32) Benzene-d6	8.270	84	856236	16.357	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	65.440%	
36) 1,2-Dichloropropane-d6	9.270	67	270742	17.518	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	70.080%	
41) Toluene-d8	10.319	98	757757	16.036	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	64.160%	
43) trans-1,3-Dichloroprop...	10.575	79	110259	17.373	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	69.480%	
47) 2-Hexanone-d5	10.922	63	96946	61.467	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	122.940%	
56) 1,1,2,2-Tetrachloroeth...	12.684	84	239795	25.371	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	101.480%	
66) 1,2-Dichlorobenzene-d4	13.849	152	248740	18.528	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	74.120%#	
Target Compounds						
13) Acetone	4.155	43	28698m	15.813	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031657.D
Acq On : 30 Jan 2025 15:21
Operator : SY/MD
Sample : Q1189-08RE
Misc : 9.50g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44R1RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/31/2025
Supervised By :Mahesh Dadoda 01/31/2025

Quant Time: Jan 31 07:35:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

