




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031665.D
Acq On : 30 Jan 2025 18:34
Operator : SY/MD
Sample : Q1189-03RE
Misc : 15.93g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/31/2025
Supervised By :Mahesh Dadoda 01/31/2025

Quant Time: Jan 31 07:37:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

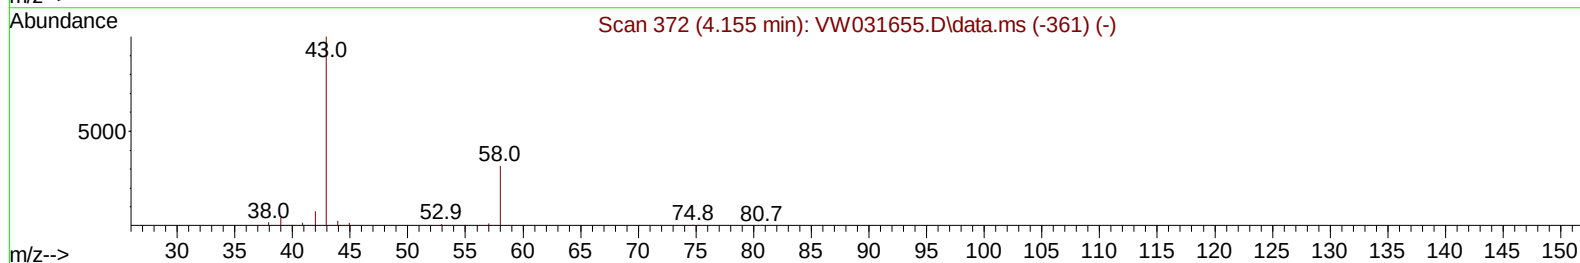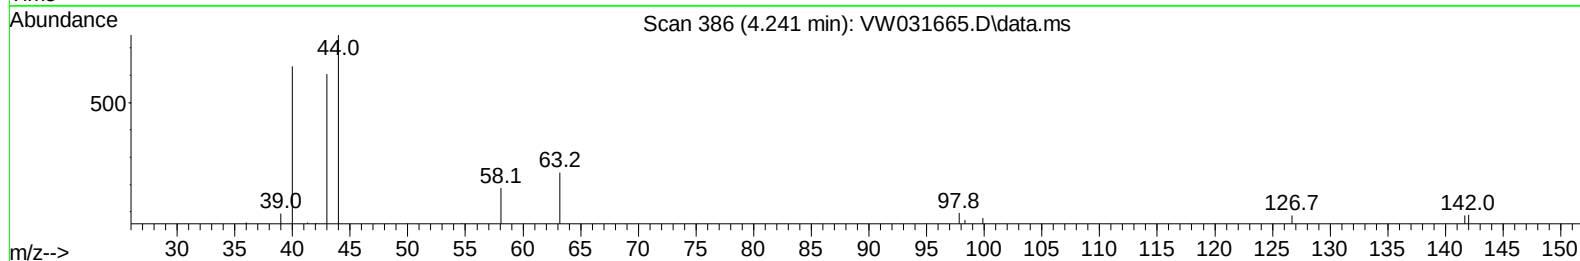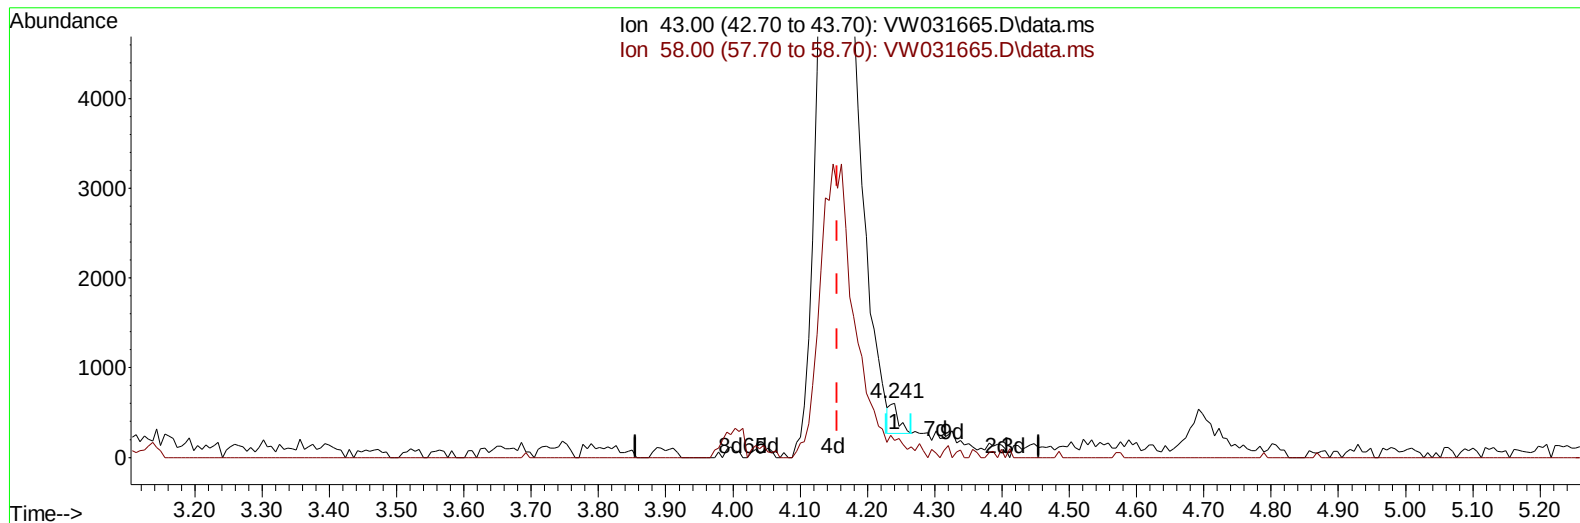

TIC: VW031665.D\data.ms

(13) Acetone (T)

4.241min (+ 0.086) 0.40 ug/L

response 326

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	25.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031665.D
Acq On : 30 Jan 2025 18:34
Operator : SY/MD
Sample : Q1189-03RE
Misc : 15.93g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q6RE

Manual IntegrationsAPPROVED

Quant Time: Jan 31 07:37:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/31/2025
Supervised By :Mahesh Dadoda 01/31/2025

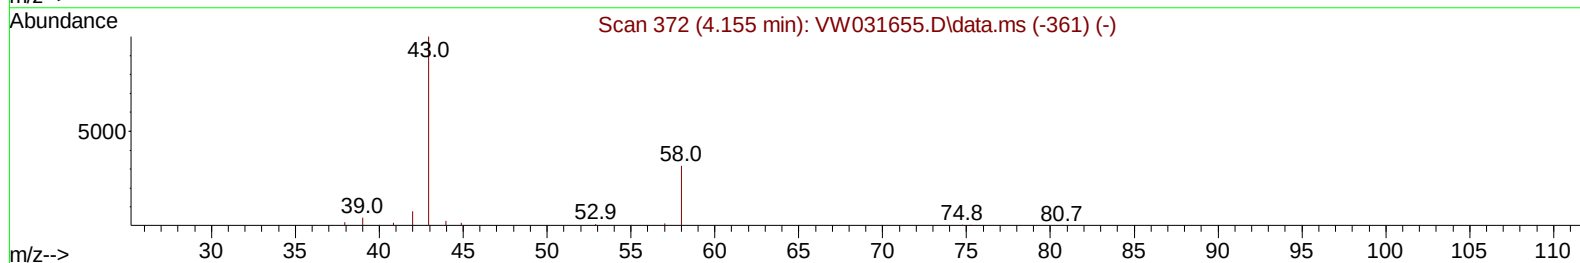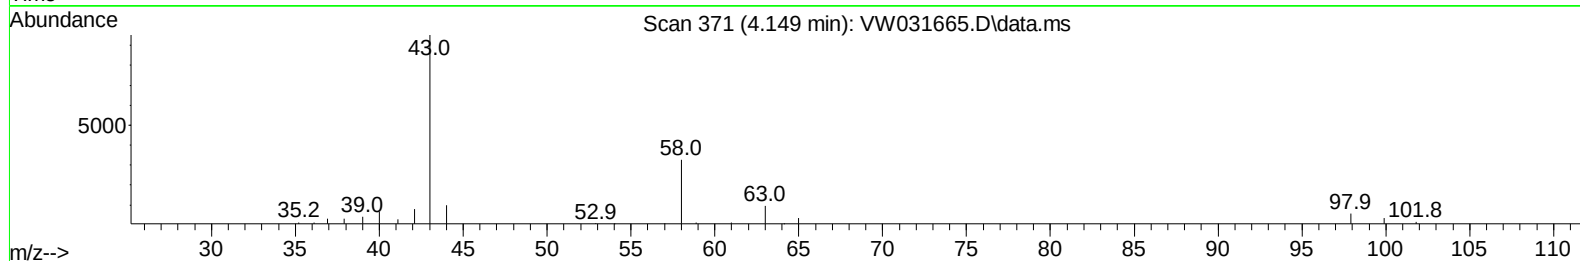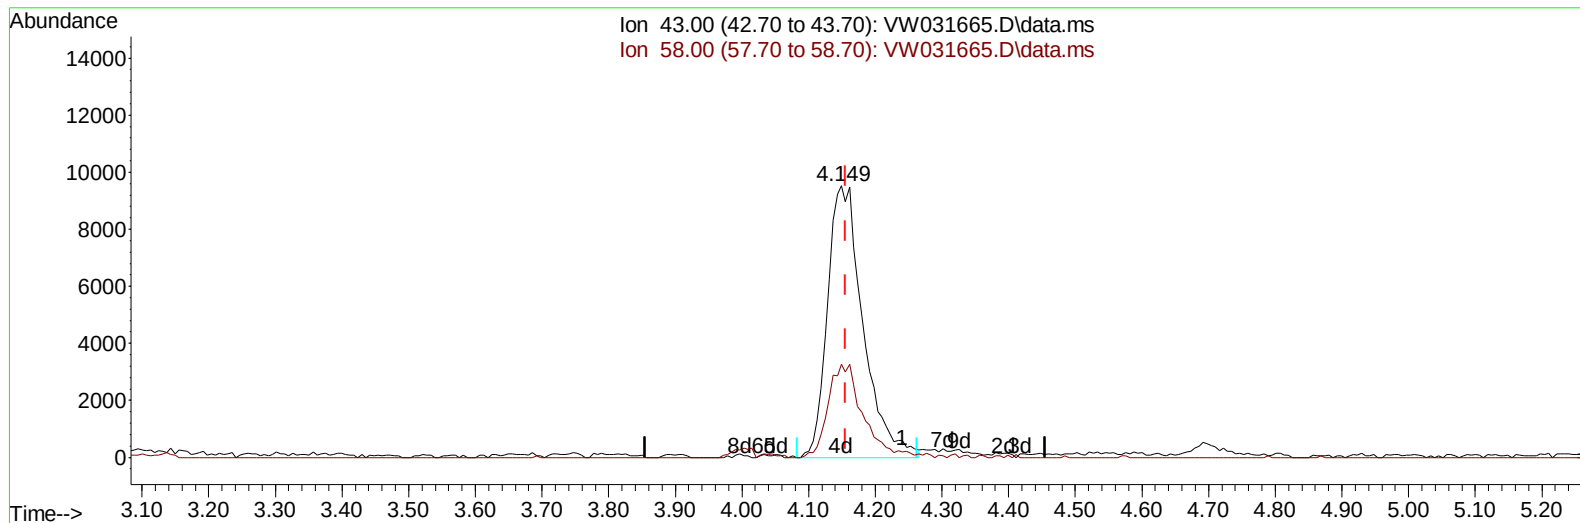

TIC: VW031665.D\data.ms

(13) Acetone (T)

4.149min (-0.006) 43.67 ug/L m

response 35359

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.24
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
 Data File : VW031665.D
 Acq On : 30 Jan 2025 18:34
 Operator : SY/MD
 Sample : Q1189-03RE
 Misc : 15.93g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44Q6RE

Manual IntegrationsAPPROVED

Quant Time: Jan 31 07:37:43 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 31 07:33:50 2025
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/31/2025
 Supervised By :Mahesh Dadoda 01/31/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	417044	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	282251	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	69078	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	95938	14.660	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.640%	
7) Chloroethane-d5	2.899	69	75704	16.198	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	64.800%	
11) 1,1-Dichloroethene-d2	4.015	65	45514	15.631	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.520%	
21) 2-Butanone-d5	7.081	46	172828	164.287	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	328.580%#	
24) Chloroform-d	7.642	84	211195	19.568	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	78.280%	
26) 1,2-Dichloroethane-d4	8.301	65	124829	23.498	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.000%	
32) Benzene-d6	8.270	84	433396	24.445	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	97.800%	
36) 1,2-Dichloropropane-d6	9.270	67	137445	26.257	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	105.040%	
41) Toluene-d8	10.319	98	336520	21.026	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	84.120%	
43) trans-1,3-Dichloroprop...	10.575	79	40116	18.662	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	74.640%	
47) 2-Hexanone-d5	10.922	63	103207	193.199	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	386.400%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	149940	46.839	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	187.360%#	
66) 1,2-Dichlorobenzene-d4	13.849	152	55593	22.945	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.800%	
Target Compounds						
13) Acetone	4.149	43	35359m	43.673	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031665.D
Acq On : 30 Jan 2025 18:34
Operator : SY/MD
Sample : Q1189-03RE
Misc : 15.93g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/31/2025
Supervised By :Mahesh Dadoda 01/31/2025

Quant Time: Jan 31 07:37:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

