

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
 Data File : VW031664.D
 Acq On : 30 Jan 2025 18:10
 Operator : SY/MD
 Sample : Q1189-02RE
 Misc : 16.80g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44Q5RE

Quant Time: Jan 31 07:37:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 31 07:33:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	415628	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.623	117	277303	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	70465	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	89493	13.722	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.880%
7) Chloroethane-d5	2.893	69	73508	15.782	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.120%
11) 1,1-Dichloroethene-d2	4.015	65	42684	14.709	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.840%
21) 2-Butanone-d5	7.081	46	178211	169.982	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	339.960%#
24) Chloroform-d	7.648	84	215680	20.051	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.200%
26) 1,2-Dichloroethane-d4	8.301	65	137457	25.963	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.840%
32) Benzene-d6	8.270	84	435227	24.986	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.960%
36) 1,2-Dichloropropane-d6	9.270	67	141485	27.511	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.040%
41) Toluene-d8	10.319	98	337118	21.439	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.760%
43) trans-1,3-Dichloroprop...	10.575	79	43129	20.422	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.680%
47) 2-Hexanone-d5	10.922	63	111751	212.926	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	425.860%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	162655	51.717	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	206.880%#
66) 1,2-Dichlorobenzene-d4	13.848	152	52514	21.248	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.000%
Target Compounds					Qvalue	
13) Acetone	4.149	43	67169	83.245	ug/L #	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013025\
Data File : VW031664.D
Acq On : 30 Jan 2025 18:10
Operator : SY/MD
Sample : Q1189-02RE
Misc : 16.80g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44Q5RE

Quant Time: Jan 31 07:37:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 31 07:33:50 2025
Response via : Initial Calibration

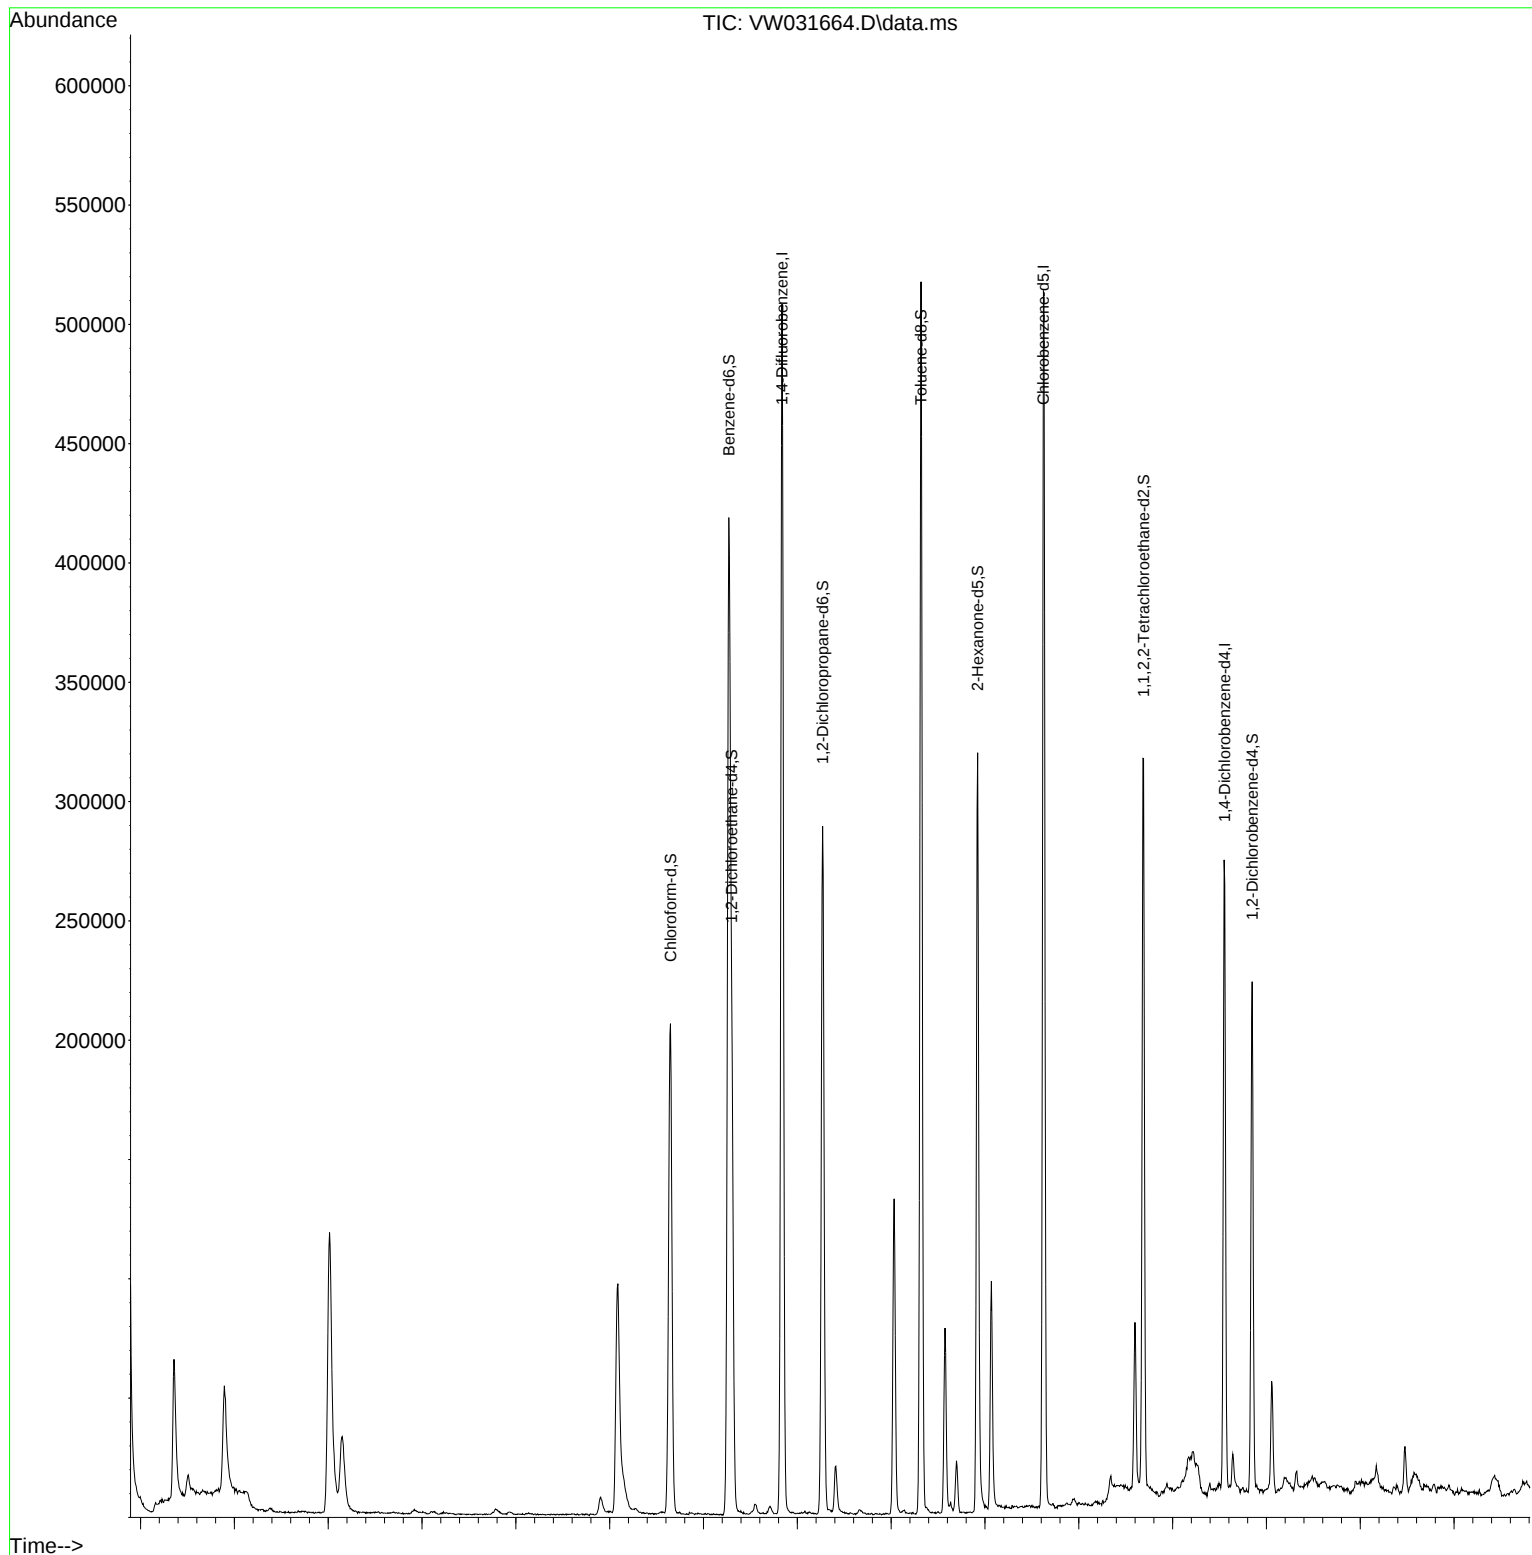

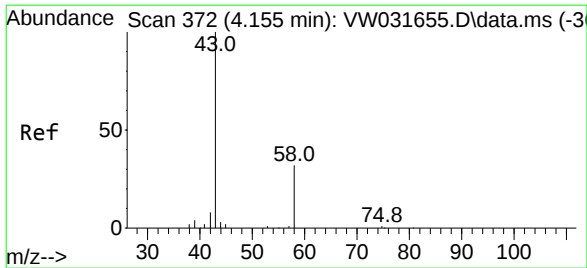

#13
 Acetone
 Concen: 83.245 ug/L
 RT: 4.149 min Scan# 371
 Delta R.T. -0.006 min
 Lab File: VW031664.D
 Acq: 30 Jan 2025 18:10

Instrument :
 MSVOA_W
 ClientSampleId :
 A44Q5RE

Tgt Ion: 43 Resp: 67169
 Ion Ratio Lower Upper
 43 100
 58 32.2 0.0 28.2#

