

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013124\
 Data File : VW027872.D
 Acq On : 31 Jan 2024 12:28
 Operator : SY/MD
 Sample : P1293-03
 Misc : 4.58g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Feb 01 00:35:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 01 00:34:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	540768	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	486995	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	249854	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	109453	16.583	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.320%
7) Chloroethane-d5	2.899	69	86906	15.019	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.080%
11) 1,1-Dichloroethene-d2	4.021	65	51213	17.249	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.000%
21) 2-Butanone-d5	7.087	46	55661	50.999	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.000%
24) Chloroform-d	7.648	84	270270	20.669	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.680%
26) 1,2-Dichloroethane-d4	8.306	65	131764	22.241	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.960%
32) Benzene-d6	8.276	84	565819	20.471	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.880%
36) 1,2-Dichloropropane-d6	9.276	67	162064	21.194	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.760%
41) Toluene-d8	10.324	98	528180	20.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.760%
43) trans-1,3-Dichloroprop...	10.574	79	67071	22.565	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.240%
47) 2-Hexanone-d5	10.922	63	51849	51.656	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	132764	24.372	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.480%
66) 1,2-Dichlorobenzene-d4	13.854	152	195049	22.207	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.840%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	4360	0.437	ug/L	Qvalue # 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013124\
Data File : VW027872.D
Acq On : 31 Jan 2024 12:28
Operator : SY/MD
Sample : P1293-03
Misc : 4.58g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Feb 01 00:35:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 01 00:34:16 2024
Response via : Initial Calibration

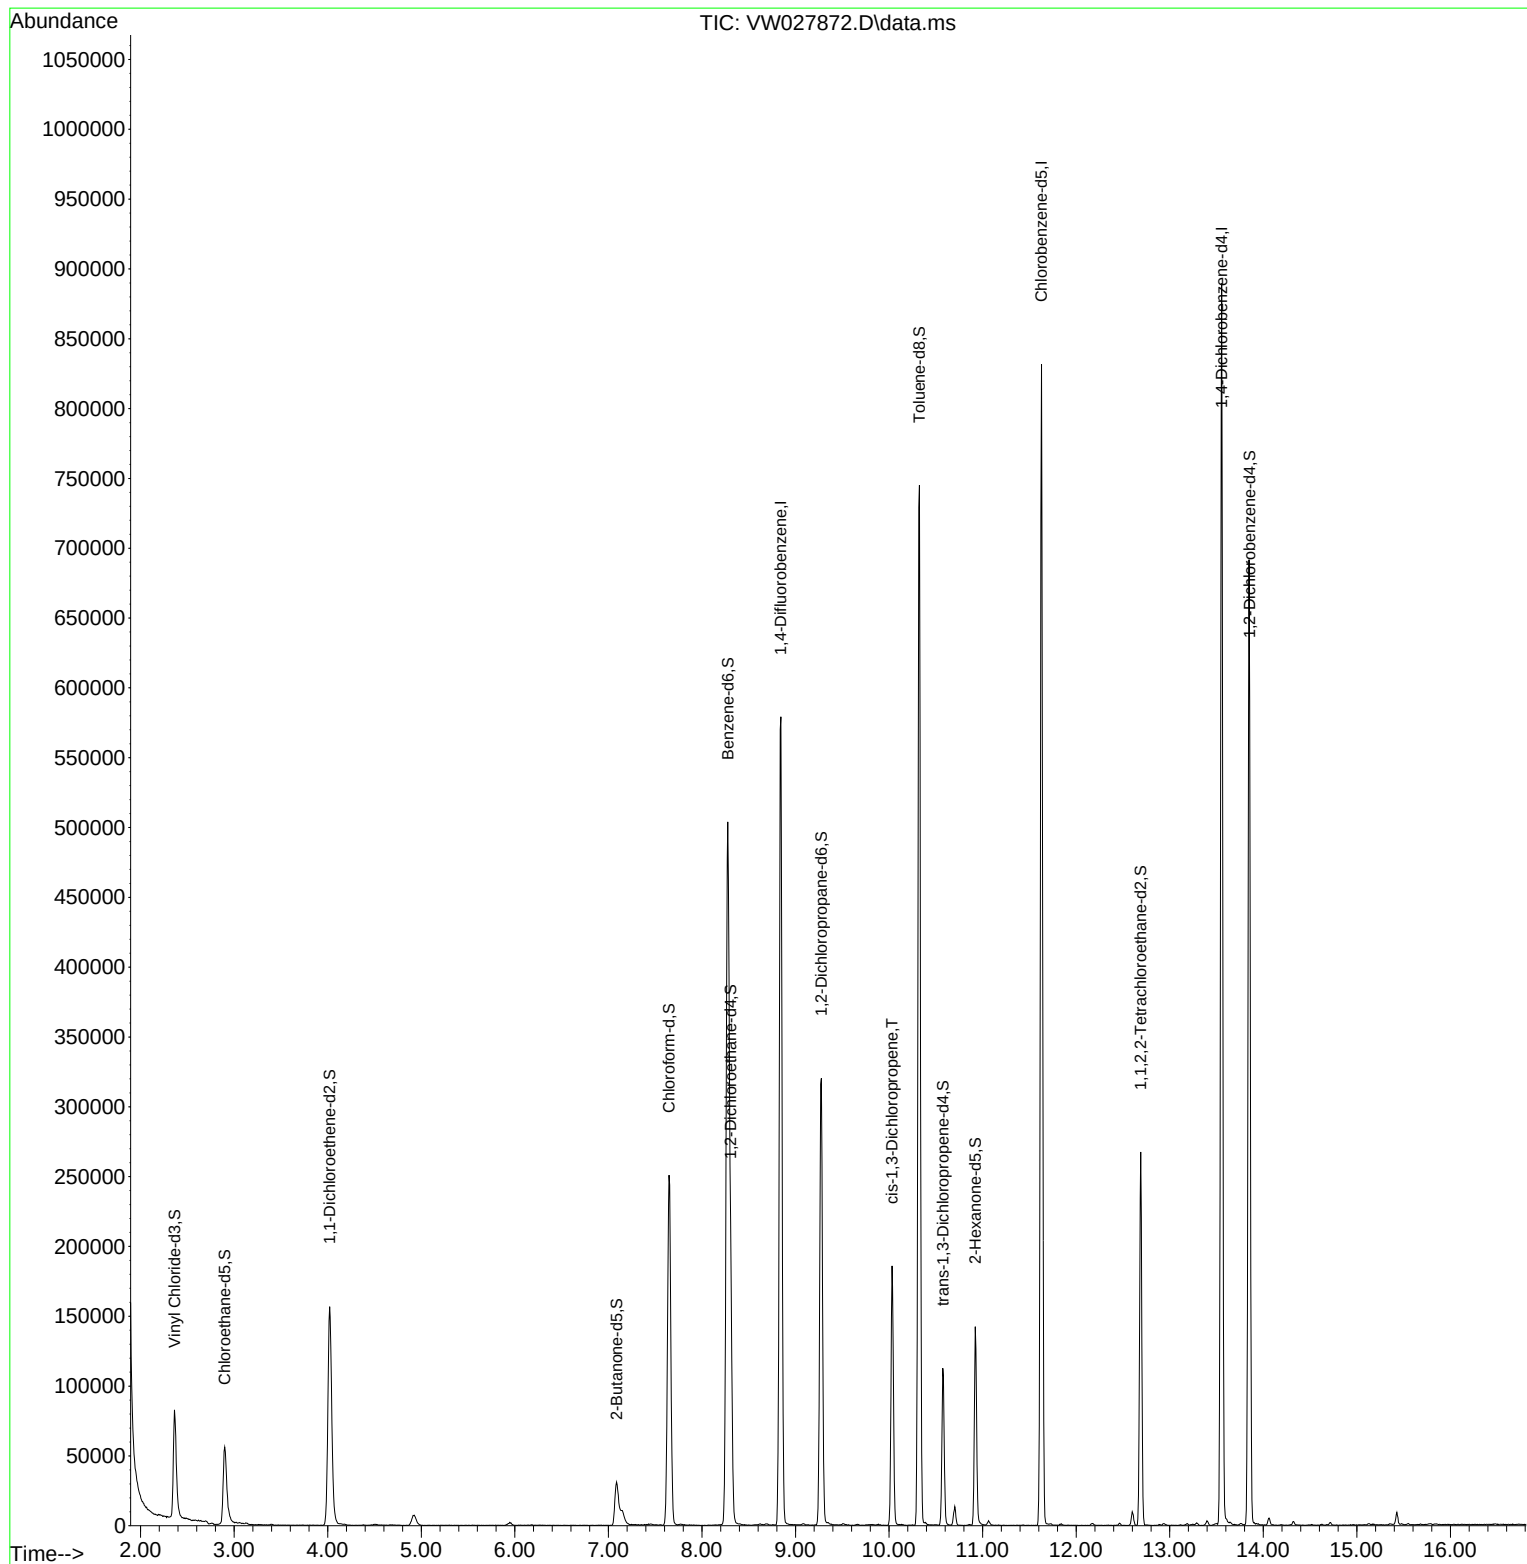

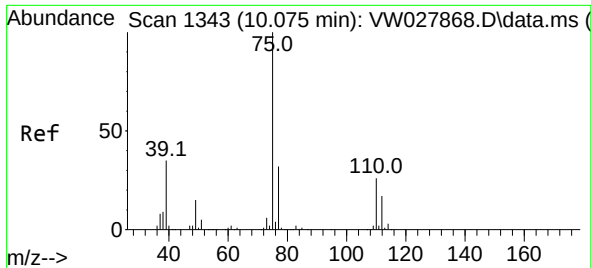

#39
 cis-1,3-Dichloropropene
 Concen: 0.437 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW027872.D
 Acq: 31 Jan 2024 12:28

Instrument :
 MSVOA_W
 ClientSampleId :

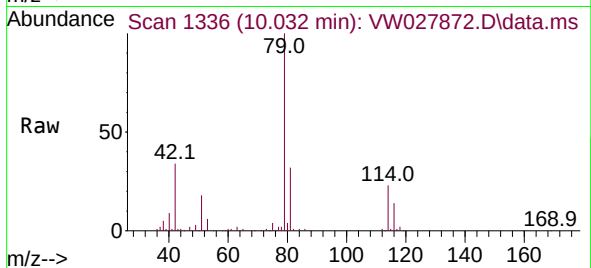

Tgt Ion: 75 Resp: 4360
 Ion Ratio Lower Upper
 75 100
 77 54.6 21.7 40.3#

