


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW013124\
Data File : VW027867.D
Acq On : 31 Jan 2024 09:26
Operator : SY/MD
Sample : BFB429
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB429

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Title : SFAM01.0
Last Update : Thu Feb 01 00:34:16 2024

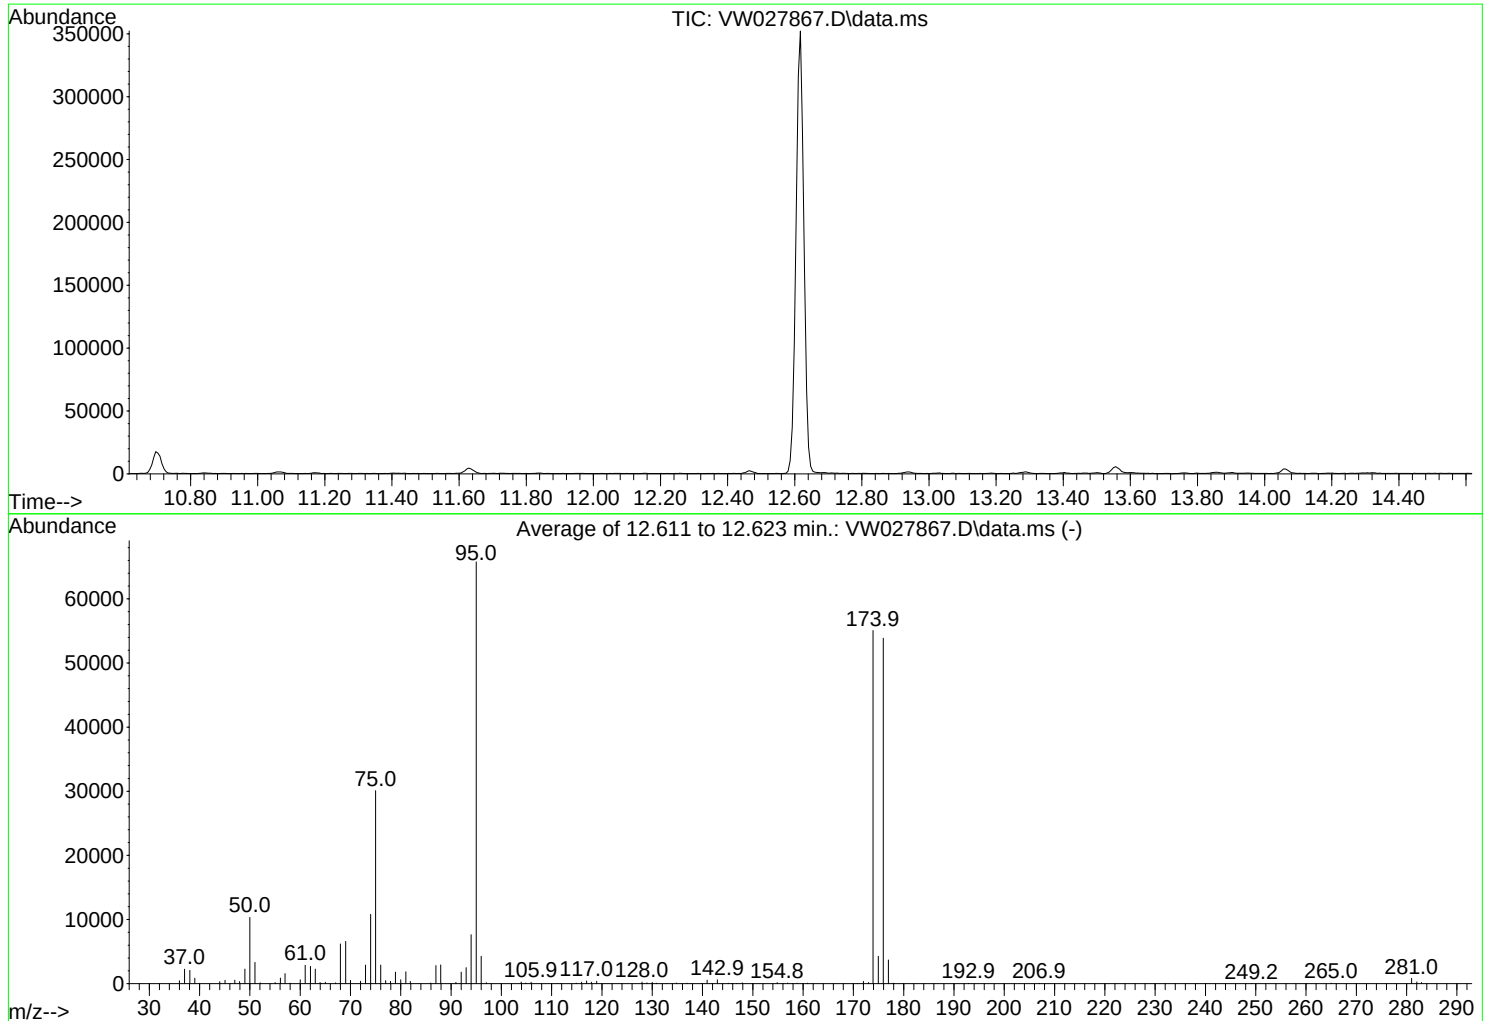

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	10340	PASS
75	95	30	80	45.7	30083	PASS
95	95	100	100	100.0	65776	PASS
96	95	5	9	6.5	4279	PASS
173	174	0.00	2	0.3	184	PASS
174	95	50	120	83.7	55067	PASS
175	174	5	9	7.8	4273	PASS
176	174	95	101	97.8	53861	PASS
177	176	5	9	6.9	3699	PASS

m/z	Abundance
40.00	168.0
43.90	121.0

Instrument :
MSVOA_W
ClientSampleId :
BFB429

m/z	Abundance
36.00	467.0
37.00	2459.0
38.00	2552.0
39.00	885.0
40.10	263.0
44.10	334.0
45.00	540.0
46.20	78.0
47.10	534.0
48.00	369.0
49.00	2443.0
50.00	11336.0
51.00	3703.0
52.10	153.0
55.00	176.0
56.10	871.0
57.00	1515.0
58.00	100.0
60.00	615.0
61.00	2938.0
62.10	2833.0
63.00	2305.0
63.90	272.0
65.00	280.0
67.10	101.0
68.00	6752.0
69.00	7222.0
70.00	479.0
72.00	329.0
73.00	3122.0
74.00	11308.0
75.00	31880.0
76.00	3193.0
77.00	438.0
78.00	418.0
79.00	1812.0
80.00	609.0
81.00	2034.0
81.90	367.0
86.00	122.0
87.00	3121.0
87.90	2818.0
90.90	180.0
92.00	1738.0
93.00	2565.0
94.00	8058.0
95.00	70624.0
96.00	4283.0
97.00	72.0
104.00	250.0
104.80	96.0
106.00	286.0
111.10	73.0
114.90	79.0
116.00	206.0
117.00	439.0
117.90	267.0
118.90	440.0
128.00	266.0
128.90	117.0
130.00	155.0
131.00	68.0
132.90	78.0
135.00	85.0
136.90	82.0
140.90	613.0
142.90	634.0
145.10	116.0
145.80	63.0
146.80	90.0
147.90	86.0
150.00	72.0
154.80	189.0
156.90	99.0
157.90	57.0
158.80	93.0
160.80	85.0
170.80	73.0
172.00	408.0
173.90	47272.0
174.90	3961.0
175.90	52248.0
177.00	3215.0
177.90	133.0
192.90	104.0
207.00	99.0
249.20	58.0
265.00	131.0
281.10	1205.0
282.10	430.0
283.00	224.0

Instrument :
MSVOA_W
ClientSampleId :
BFB429

m/z	Abundance
36.00	494.0
37.00	2439.0
38.10	2189.0
39.00	935.0
40.00	177.0
44.00	465.0
45.00	643.0
47.00	663.0
47.90	382.0
49.00	2549.0
50.00	11472.0
51.00	3867.0
52.00	159.0
55.00	185.0
56.00	1028.0
57.00	1895.0
58.00	94.0
60.00	686.0
61.00	3237.0
62.00	2993.0
63.00	2667.0
64.00	278.0
65.00	279.0
67.00	123.0
68.00	6851.0
69.10	7155.0
70.00	553.0
72.00	356.0
73.00	3210.0
74.00	12499.0
75.00	33360.0
76.00	3196.0
77.00	624.0
77.80	302.0
78.90	2058.0
80.00	624.0
81.00	1982.0
81.90	396.0
85.90	103.0
87.00	3044.0
87.90	3123.0
91.00	232.0
92.00	2151.0
93.00	2719.0
94.00	8645.0
95.00	74232.0
96.00	5111.0
97.00	200.0
103.90	263.0
104.90	144.0
105.80	227.0
111.80	64.0
114.90	91.0
116.00	255.0
116.90	500.0
117.90	196.0
118.90	346.0
127.90	287.0
129.00	148.0
130.00	280.0
130.90	94.0
134.80	141.0
136.90	147.0
139.90	59.0
140.90	544.0
142.90	685.0
145.10	95.0
145.80	55.0
147.90	231.0
154.80	203.0
156.90	113.0
158.80	126.0
160.90	83.0
172.00	380.0
173.00	552.0
173.90	62200.0
174.90	4394.0
176.00	60856.0
176.90	4306.0
177.90	89.0
192.90	62.0
206.90	57.0
265.00	87.0
281.00	808.0
282.00	253.0
282.90	195.0

Instrument :
MSVOA_W
ClientSampleId :
BFB429

m/z	Abundance
36.00	401.0
37.00	1820.0
38.00	1510.0
39.10	706.0
39.90	217.0
44.00	436.0
45.10	432.0
46.90	467.0
48.00	220.0
49.00	1821.0
50.00	8213.0
51.00	2395.0
52.00	84.0
55.00	149.0
56.00	761.0
57.00	1308.0
58.00	59.0
60.00	496.0
61.00	2406.0
62.00	2229.0
63.00	1859.0
64.20	140.0
65.00	132.0
67.00	152.0
68.00	4940.0
69.00	5355.0
70.00	503.0
72.00	441.0
73.00	2358.0
74.00	8606.0
75.00	25008.0
76.00	2289.0
77.00	356.0
78.00	302.0
78.90	1553.0
80.00	530.0
81.00	1505.0
81.90	326.0
86.00	88.0
87.00	2270.0
88.00	2801.0
91.00	210.0
92.00	1484.0
93.00	2217.0
94.00	6233.0
95.00	52472.0
96.00	3443.0
97.00	147.0
103.90	255.0
104.80	79.0
105.90	186.0
111.80	53.0
114.90	96.0
115.90	221.0
116.90	330.0
117.90	237.0
119.00	326.0
123.90	62.0
127.90	180.0
128.90	83.0
130.00	149.0
130.80	80.0
134.80	118.0
140.90	488.0
141.90	55.0
143.00	499.0
146.00	67.0
147.80	100.0
154.90	131.0
156.00	57.0
157.00	85.0
160.90	87.0
172.10	249.0
173.90	55728.0
175.00	4465.0
175.90	48480.0
177.00	3576.0
178.10	62.0
280.90	441.0
282.00	143.0
282.90	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB429