

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020124\
 Data File : VW027901.D
 Acq On : 01 Feb 2024 13:29
 Operator : SY/MD
 Sample : P1303-10
 Misc : 4.88g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0FJ2

Quant Time: Feb 01 21:39:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 01 21:37:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	435253	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	398744	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	199352	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	87220	16.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.680%
7) Chloroethane-d5	2.893	69	64947	13.945	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.800%
11) 1,1-Dichloroethene-d2	4.027	65	39427	16.499	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.000%
21) 2-Butanone-d5	7.081	46	50389	57.361	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.720%
24) Chloroform-d	7.648	84	218126	20.725	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.880%
26) 1,2-Dichloroethane-d4	8.307	65	109515	22.967	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.880%
32) Benzene-d6	8.276	84	437634	19.338	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.360%
36) 1,2-Dichloropropane-d6	9.270	67	128555	20.533	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.120%
41) Toluene-d8	10.318	98	410276	19.392	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.560%
43) trans-1,3-Dichloroprop...	10.575	79	53578	22.015	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.040%
47) 2-Hexanone-d5	10.922	63	48283	58.750	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	121713	27.288	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.160%
66) 1,2-Dichlorobenzene-d4	13.848	152	154951	22.111	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.440%
Target Compounds						
16) Methylene chloride	4.923	84	19141	3.033	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020124\
Data File : VW027901.D
Acq On : 01 Feb 2024 13:29
Operator : SY/MD
Sample : P1303-10
Misc : 4.88g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0FJ2


Quant Time: Feb 01 21:39:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 01 21:37:27 2024
Response via : Initial Calibration

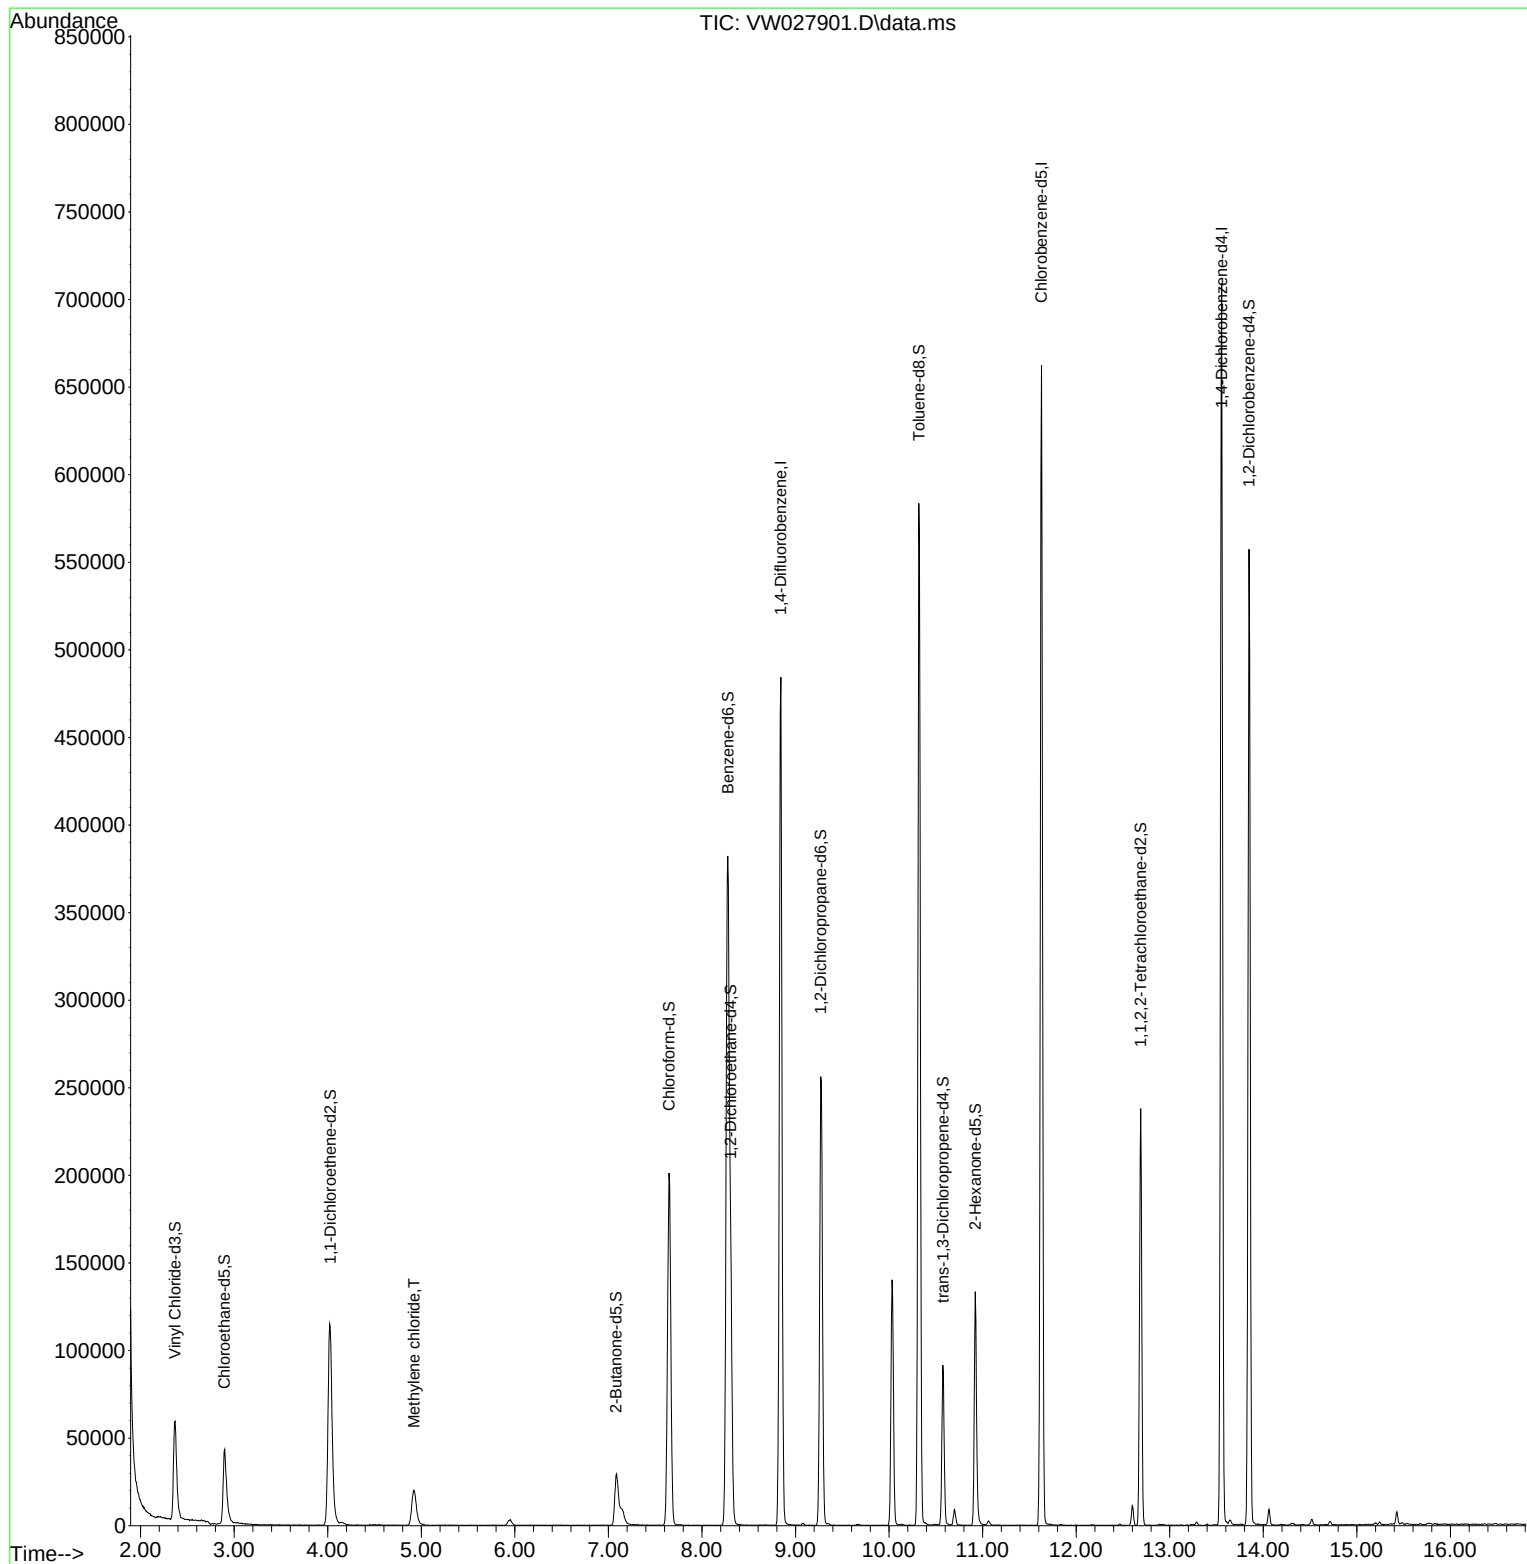

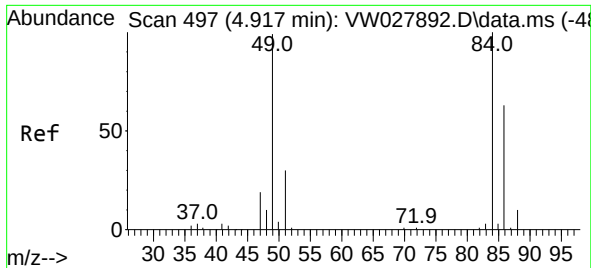

#16
Methylene chloride
Concen: 3.033 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW027901.D
Acq: 01 Feb 2024 13:29

Instrument :
MSVOA_W
ClientSampleId :
C0FJ2

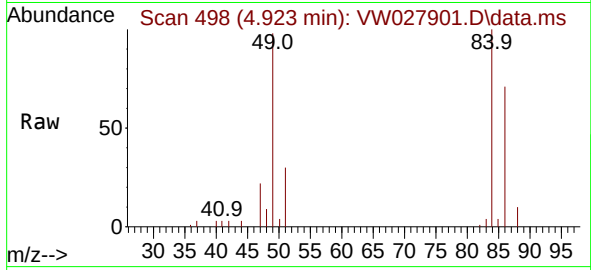

Tgt Ion:	84	Resp:	19141
Ion	Ratio	Lower	Upper
84	100		
86	70.8	43.5	80.9
49	98.0	70.3	130.5

