

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020124\
 Data File : VW027902.D
 Acq On : 01 Feb 2024 13:53
 Operator : SY/MD
 Sample : P1303-11
 Misc : 5.08g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0FJ3

Quant Time: Feb 01 21:39:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 01 21:37:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	327840	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	289192	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	132252	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	68295	17.068	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.280%
7) Chloroethane-d5	2.899	69	58928	16.798	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.200%
11) 1,1-Dichloroethene-d2	4.021	65	30899	17.167	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.680%
21) 2-Butanone-d5	7.081	46	29660	44.826	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.660%
24) Chloroform-d	7.648	84	161078	20.319	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.280%
26) 1,2-Dichloroethane-d4	8.307	65	74422	20.721	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.880%
32) Benzene-d6	8.276	84	332171	20.238	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.960%
36) 1,2-Dichloropropane-d6	9.270	67	93679	20.630	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.520%
41) Toluene-d8	10.319	98	305789	19.928	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.720%
43) trans-1,3-Dichloroprop...	10.575	79	35210	19.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.800%
47) 2-Hexanone-d5	10.922	63	25982	43.591	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.180%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	73189	22.625	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.520%
66) 1,2-Dichlorobenzene-d4	13.849	152	102418	22.030	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.120%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	14701	3.093	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020124\
Data File : VW027902.D
Acq On : 01 Feb 2024 13:53
Operator : SY/MD
Sample : P1303-11
Misc : 5.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0FJ3


Quant Time: Feb 01 21:39:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 01 21:37:27 2024
Response via : Initial Calibration

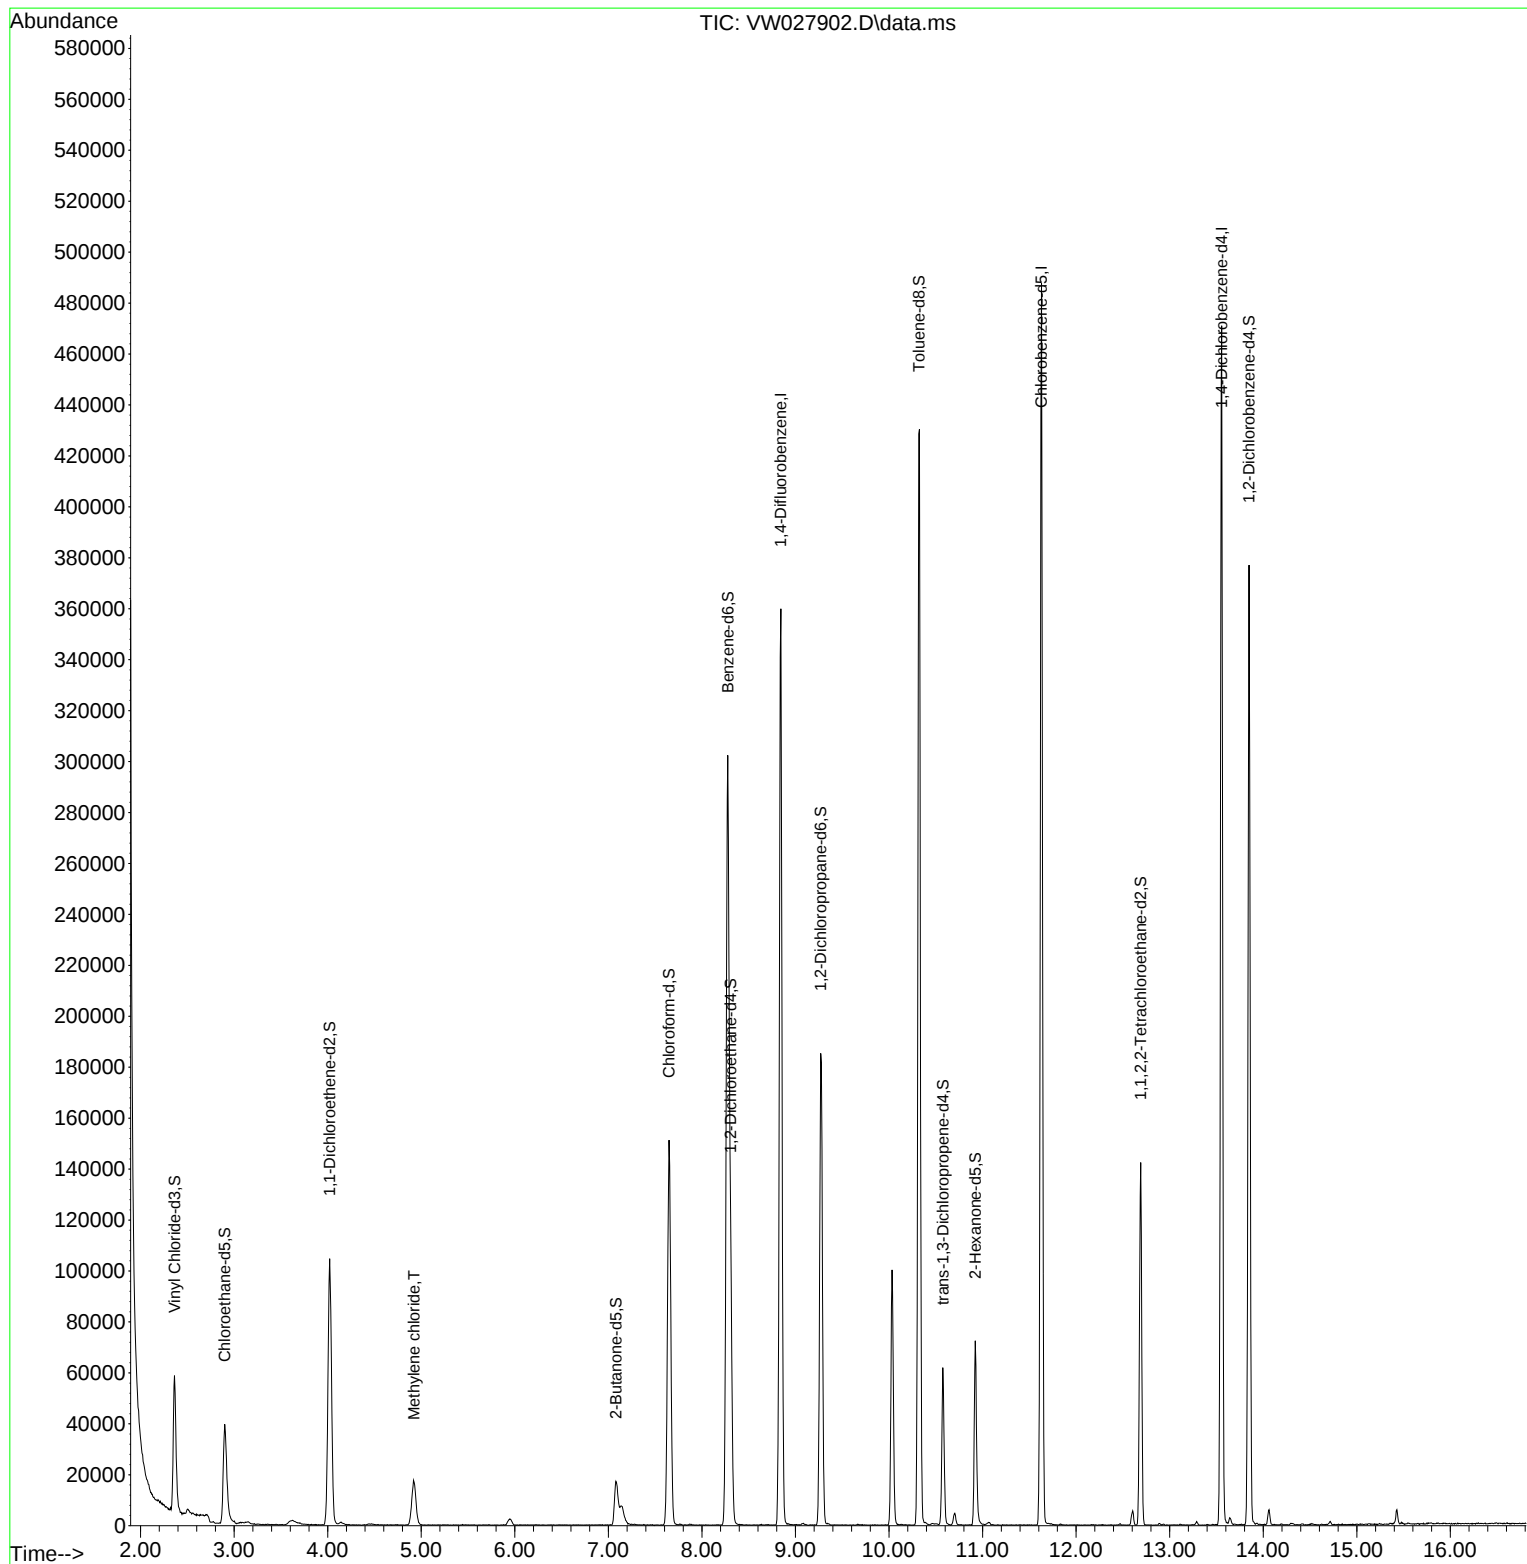

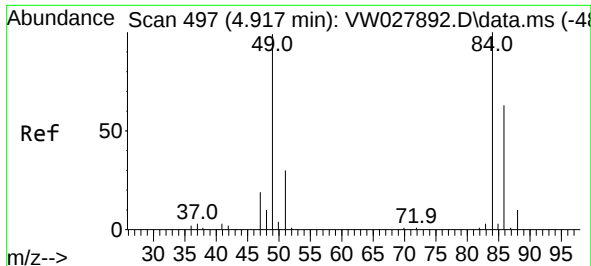

#16
Methylene chloride
Concen: 3.093 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW027902.D
Acq: 01 Feb 2024 13:53

Instrument :
MSVOA_W
ClientSampleId :
C0FJ3

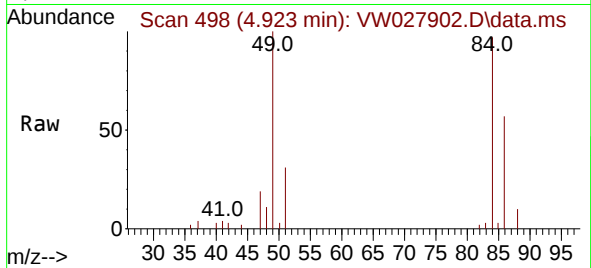

Tgt Ion: 84 Resp: 14701

Ion	Ratio	Lower	Upper
84	100		
86	58.7	43.5	80.9
49	103.6	70.3	130.5

