




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
Data File : VW027921.D
Acq On : 02 Feb 2024 11:26
Operator : SY/MD
Sample : P1293-11
Misc : 5.09g/10mL/MSVOA_W/SoIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/05/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 23:02:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 23:01:12 2024
Response via : Initial Calibration

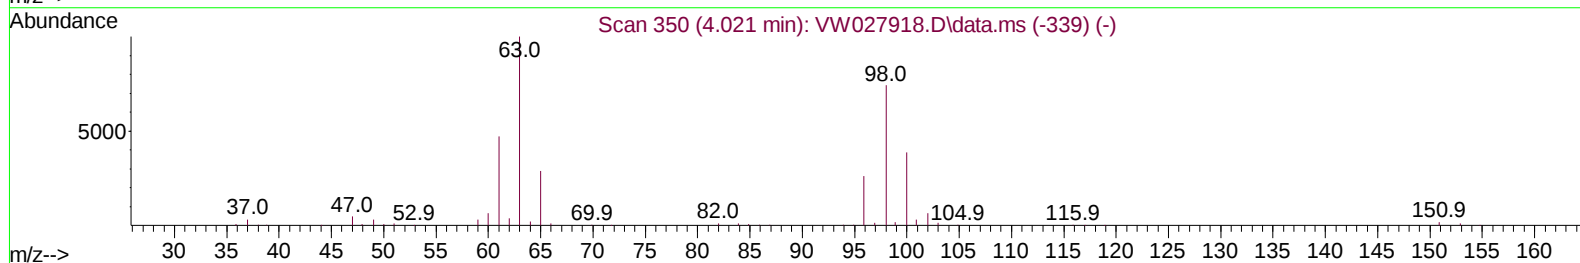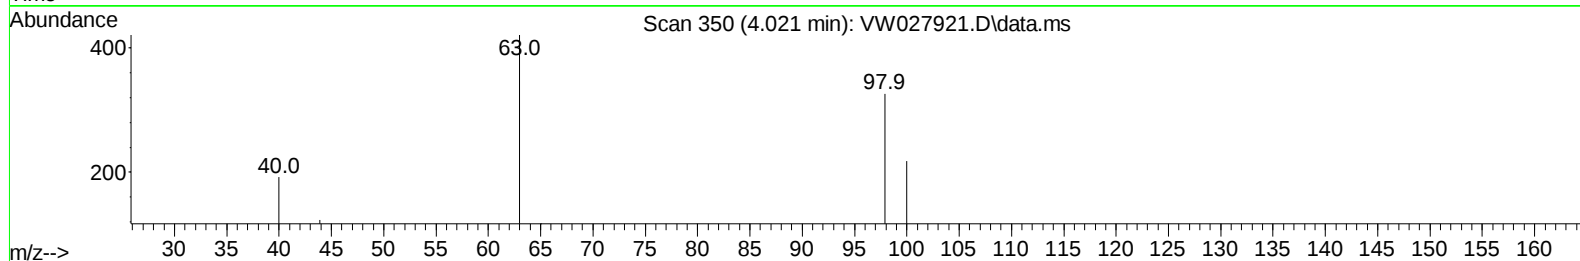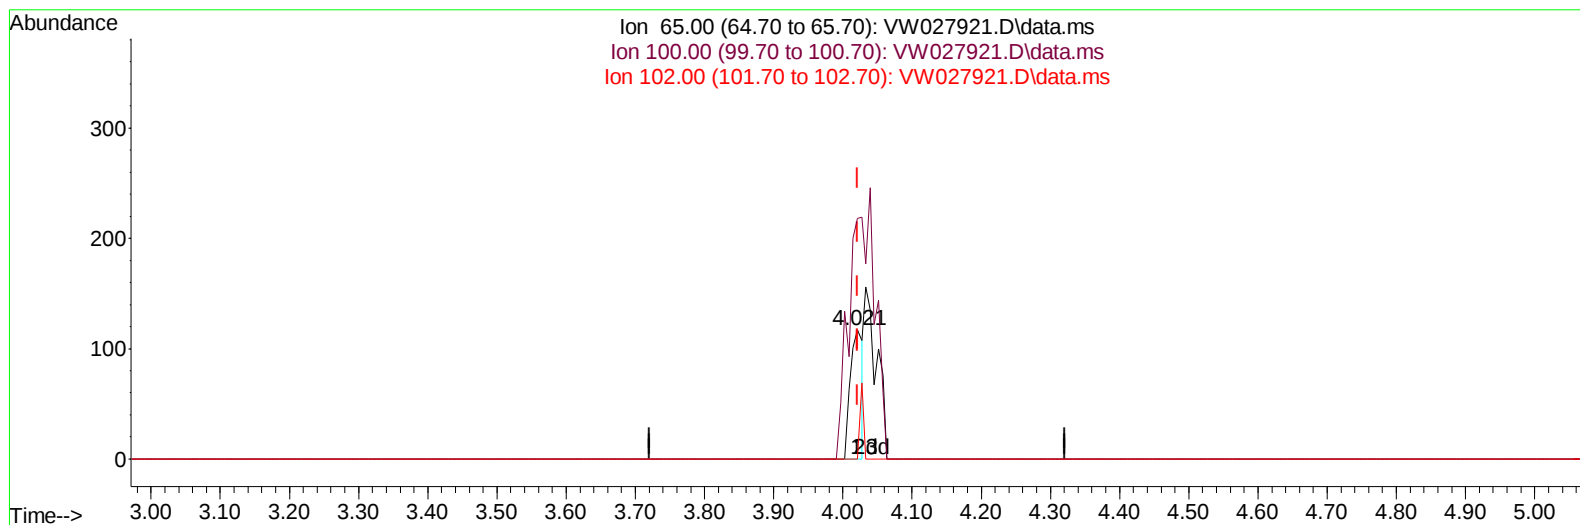

TIC: VW027921.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.000) 7.03 ug/L

response 142

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	152.50	281.69#
102.00	22.80	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
Data File : VW027921.D
Acq On : 02 Feb 2024 11:26
Operator : SY/MD
Sample : P1293-11
Misc : 5.09g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/05/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 23:02:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 23:01:12 2024
Response via : Initial Calibration

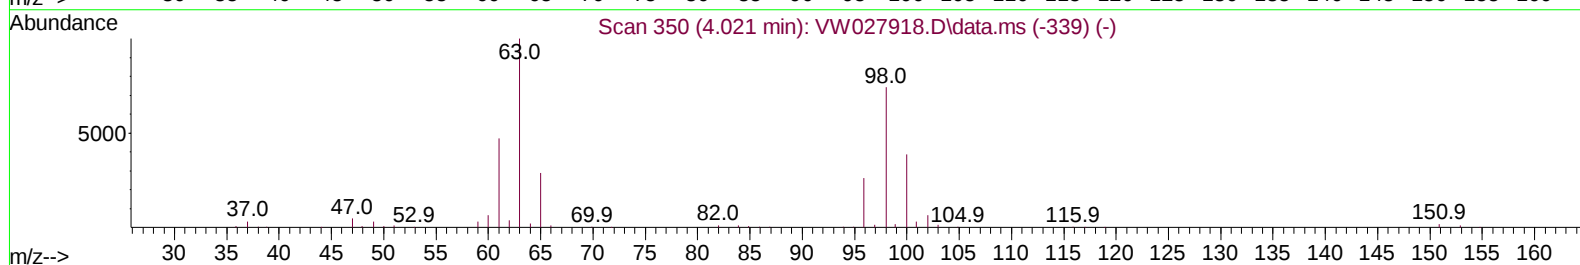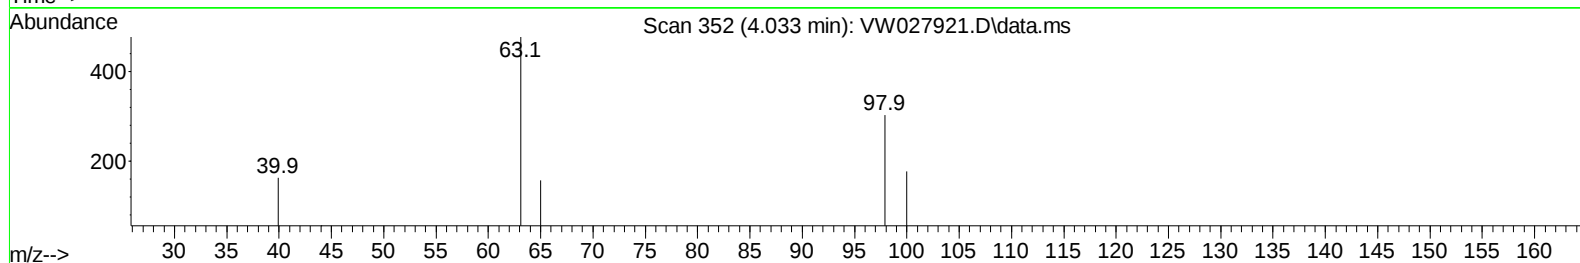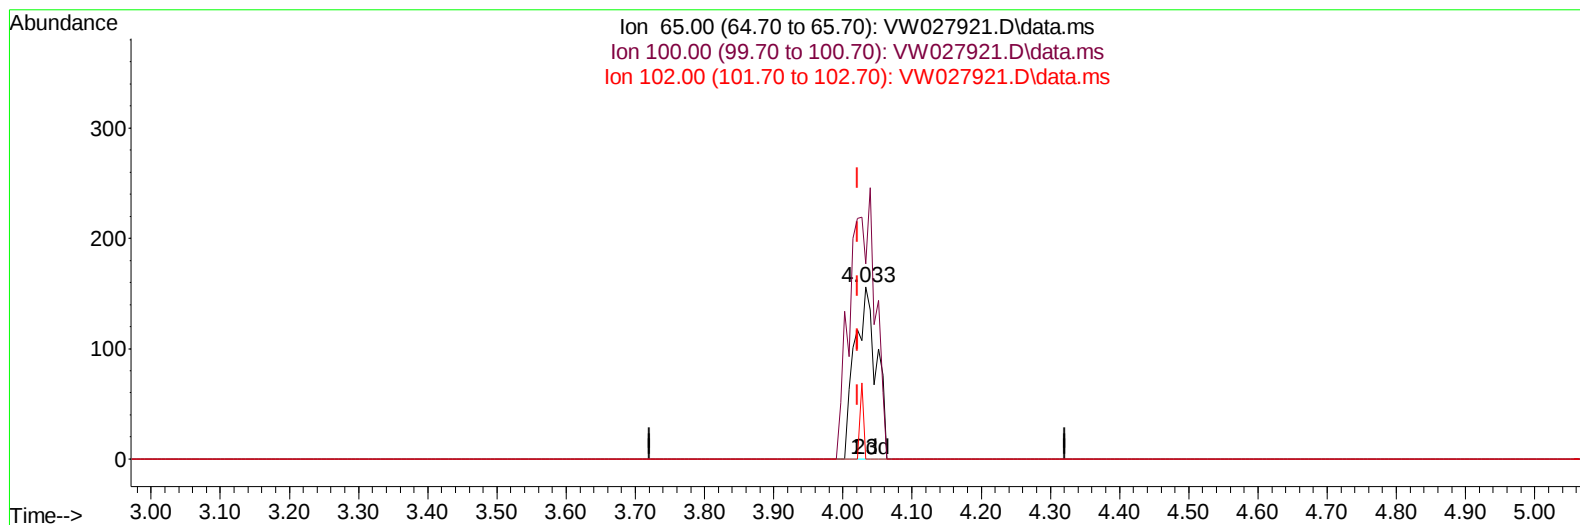

TIC: VW027921.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.033min (+ 0.012) 16.67 ug/L m

response 337

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	152.50	118.69
102.00	22.80	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
 Data File : VW027921.D
 Acq On : 02 Feb 2024 11:26
 Operator : SY/MD
 Sample : P1293-11
 Misc : 5.09g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/05/2024
 Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 23:02:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 02 23:01:12 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		3681	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		3120	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		1304	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		915	20.366	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.480%		
7) Chloroethane-d5	2.899	69		808	20.514	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	82.040%		
11) 1,1-Dichloroethene-d2	4.033	65		337m	16.675	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	66.680%		
21) 2-Butanone-d5	0.000	46		0d	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery =	0.000%#		
24) Chloroform-d	7.648	84		2190	24.604	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	98.400%		
26) 1,2-Dichloroethane-d4	8.301	65		1180	29.261	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	117.040%		
32) Benzene-d6	8.270	84		4202	23.729	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	94.920%		
36) 1,2-Dichloropropane-d6	9.270	67		1361	27.781	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	111.120%		
41) Toluene-d8	10.325	98		3982	24.054	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	96.200%		
43) trans-1,3-Dichloroprop...	10.581	79		209	10.975	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	43.920%		
47) 2-Hexanone-d5	0.000	63		0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery =	0.000%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		926	26.533	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	106.120%		
66) 1,2-Dichlorobenzene-d4	13.848	152		1002	21.859	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	87.440%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
Data File : VW027921.D
Acq On : 02 Feb 2024 11:26
Operator : SY/MD
Sample : P1293-11
Misc : 5.09g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/05/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 23:02:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 23:01:12 2024
Response via : Initial Calibration

