

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
 Data File : VW027922.D
 Acq On : 02 Feb 2024 11:50
 Operator : SY/MD
 Sample : P1303-20
 Misc : 5.81g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0FJ7

Quant Time: Feb 02 23:02:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 02 23:01:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	472585	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	412636	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	182049	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	93196	16.157	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.640%		
7) Chloroethane-d5	2.899	69	79672	15.755	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.040%		
11) 1,1-Dichloroethene-d2	4.021	65	42901	16.534	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.120%		
21) 2-Butanone-d5	7.087	46	44170	46.310	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.620%		
24) Chloroform-d	7.648	84	230252	20.149	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.600%		
26) 1,2-Dichloroethane-d4	8.307	65	110274	21.299	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.200%		
32) Benzene-d6	8.276	84	478906	20.449	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	81.800%		
36) 1,2-Dichloropropane-d6	9.270	67	133122	20.546	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	82.200%		
41) Toluene-d8	10.319	98	438617	20.033	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.120%		
43) trans-1,3-Dichloroprop...	10.575	79	51642	20.505	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.000%		
47) 2-Hexanone-d5	10.922	63	41761	49.103	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.200%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	109263	23.672	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.680%		
66) 1,2-Dichlorobenzene-d4	13.855	152	141208	22.065	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	88.280%		
Target Compounds						Qvalue
34) Trichloroethene	9.087	95	2730	0.439	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
Data File : VW027922.D
Acq On : 02 Feb 2024 11:50
Operator : SY/MD
Sample : P1303-20
Misc : 5.81g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0FJ7


Quant Time: Feb 02 23:02:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 23:01:12 2024
Response via : Initial Calibration

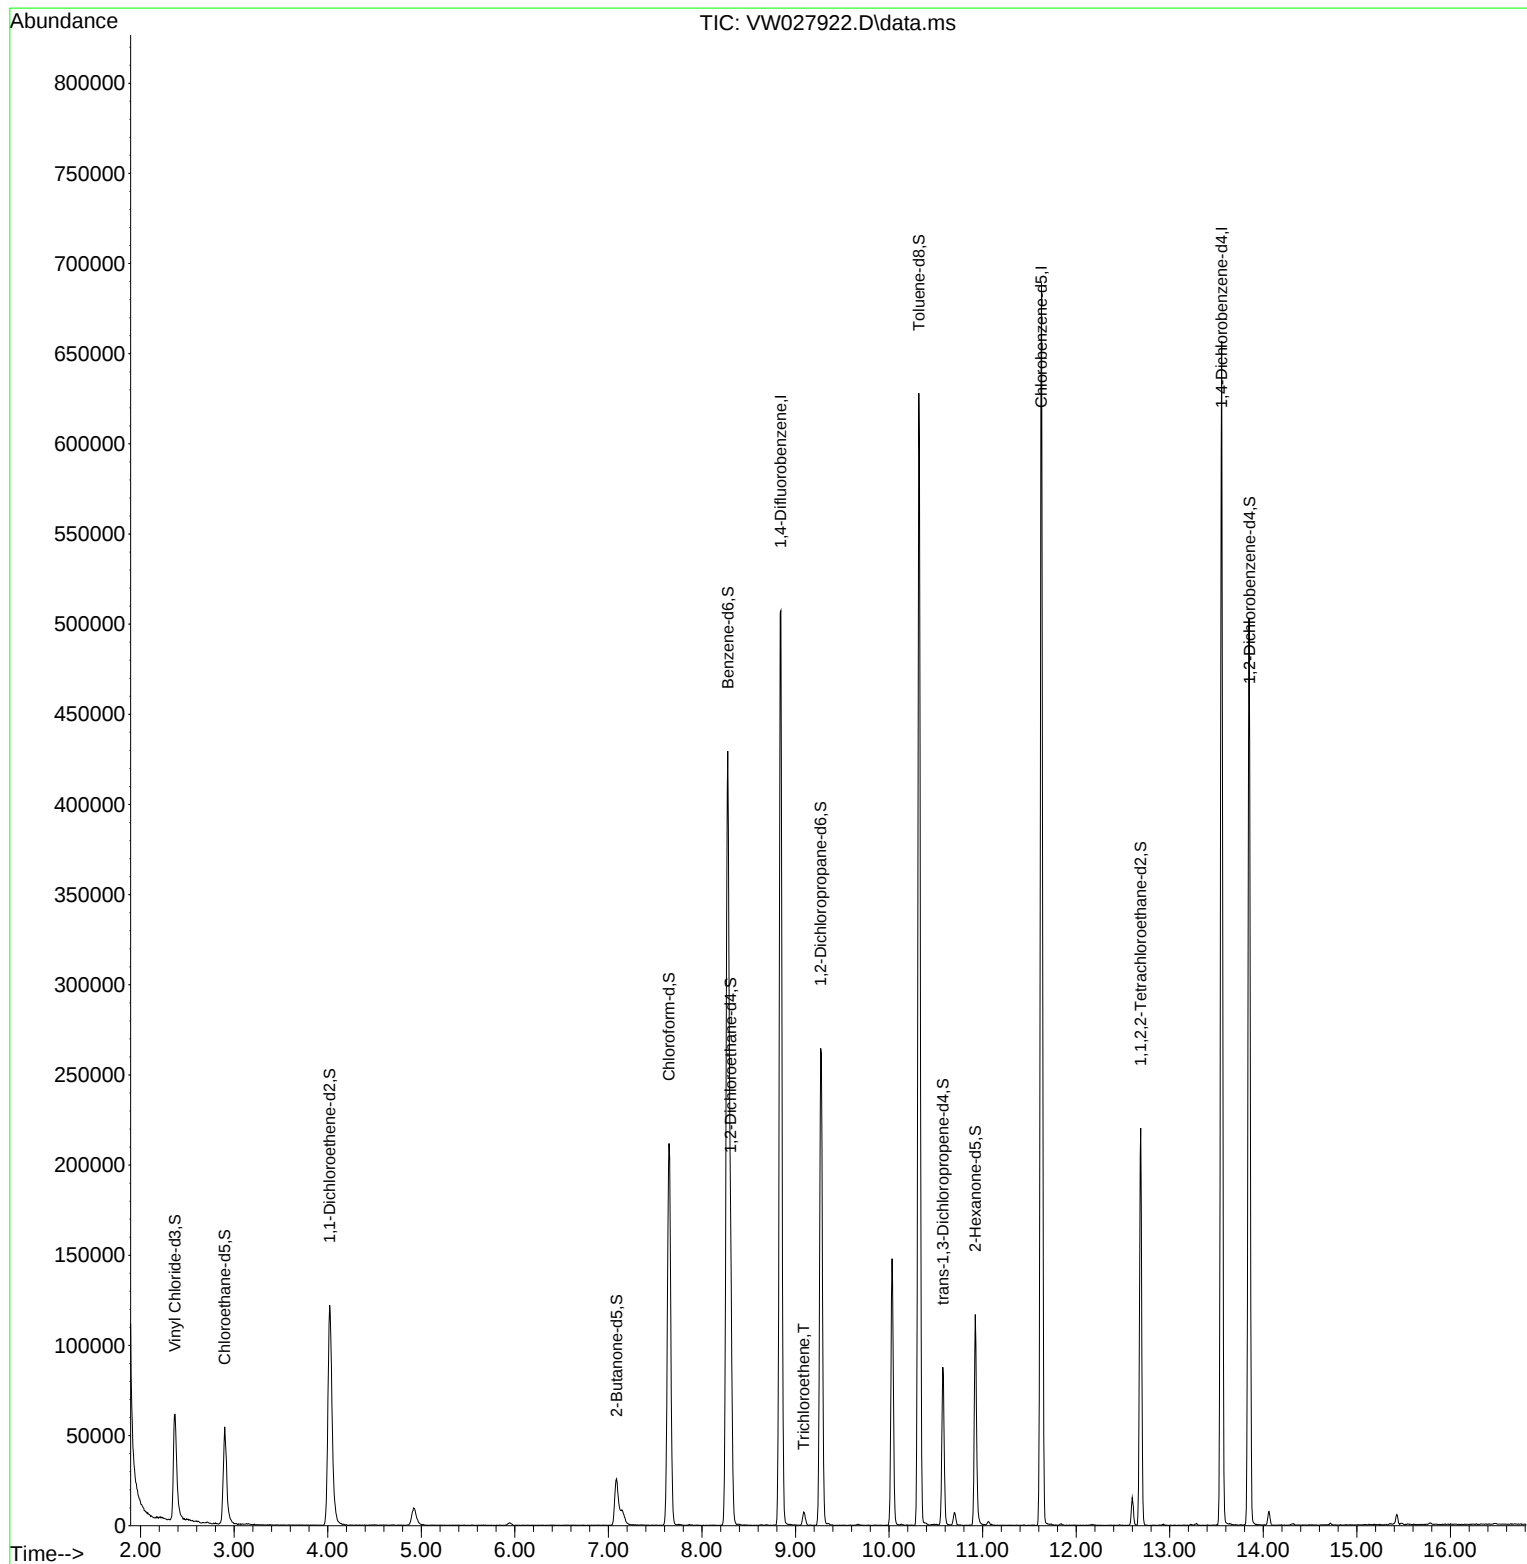

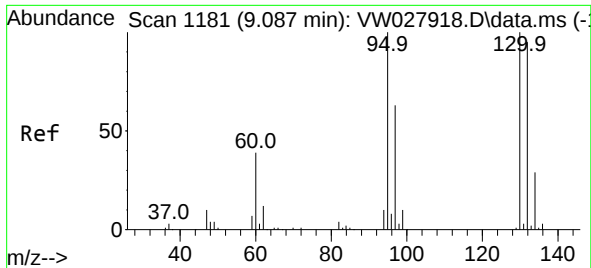

#34
 Trichloroethene
 Concen: 0.439 ug/L
 RT: 9.087 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VW027922.D
 Acq: 02 Feb 2024 11:50

Instrument :
 MSVOA_W
 ClientSampleId :
 C0FJ7

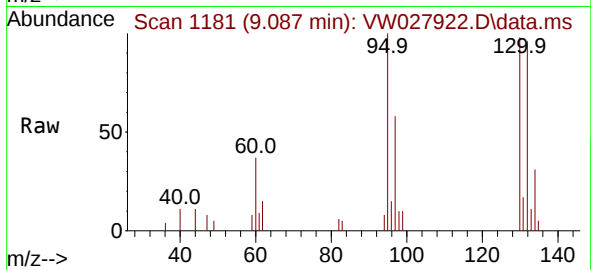

Tgt Ion:	95	Resp:	2730
Ion	Ratio	Lower	Upper
95	100		
97	57.7	45.1	83.9
132	96.2	74.1	137.5
130	97.7	73.3	136.1

