

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
 Data File : VW027940.D
 Acq On : 02 Feb 2024 19:19
 Operator : SY/MD
 Sample : P1286-11
 Misc : 4.79g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH6X5

Quant Time: Feb 02 23:06:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 02 23:01:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	202945	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	181493	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	74123	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	37312	15.064	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.240%
7) Chloroethane-d5	2.893	69	33504	15.428	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.720%
11) 1,1-Dichloroethene-d2	4.021	65	16733	15.017	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.080%
21) 2-Butanone-d5	7.075	46	24823	60.604	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.200%
24) Chloroform-d	7.648	84	99368	20.249	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.000%
26) 1,2-Dichloroethane-d4	8.300	65	52046	23.409	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.640%
32) Benzene-d6	8.276	84	196342	19.061	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.240%
36) 1,2-Dichloropropane-d6	9.270	67	59730	20.960	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.840%
41) Toluene-d8	10.318	98	181269	18.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.280%
43) trans-1,3-Dichloroprop...	10.574	79	22538	20.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.400%
47) 2-Hexanone-d5	10.922	63	21864	58.449	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	57043	28.098	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	57404	22.030	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.120%
Target Compounds						
13) Acetone	4.124	43	4391	8.388	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020224\
Data File : VW027940.D
Acq On : 02 Feb 2024 19:19
Operator : SY/MD
Sample : P1286-11
Misc : 4.79g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH6X5

Quant Time: Feb 02 23:06:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 23:01:12 2024
Response via : Initial Calibration

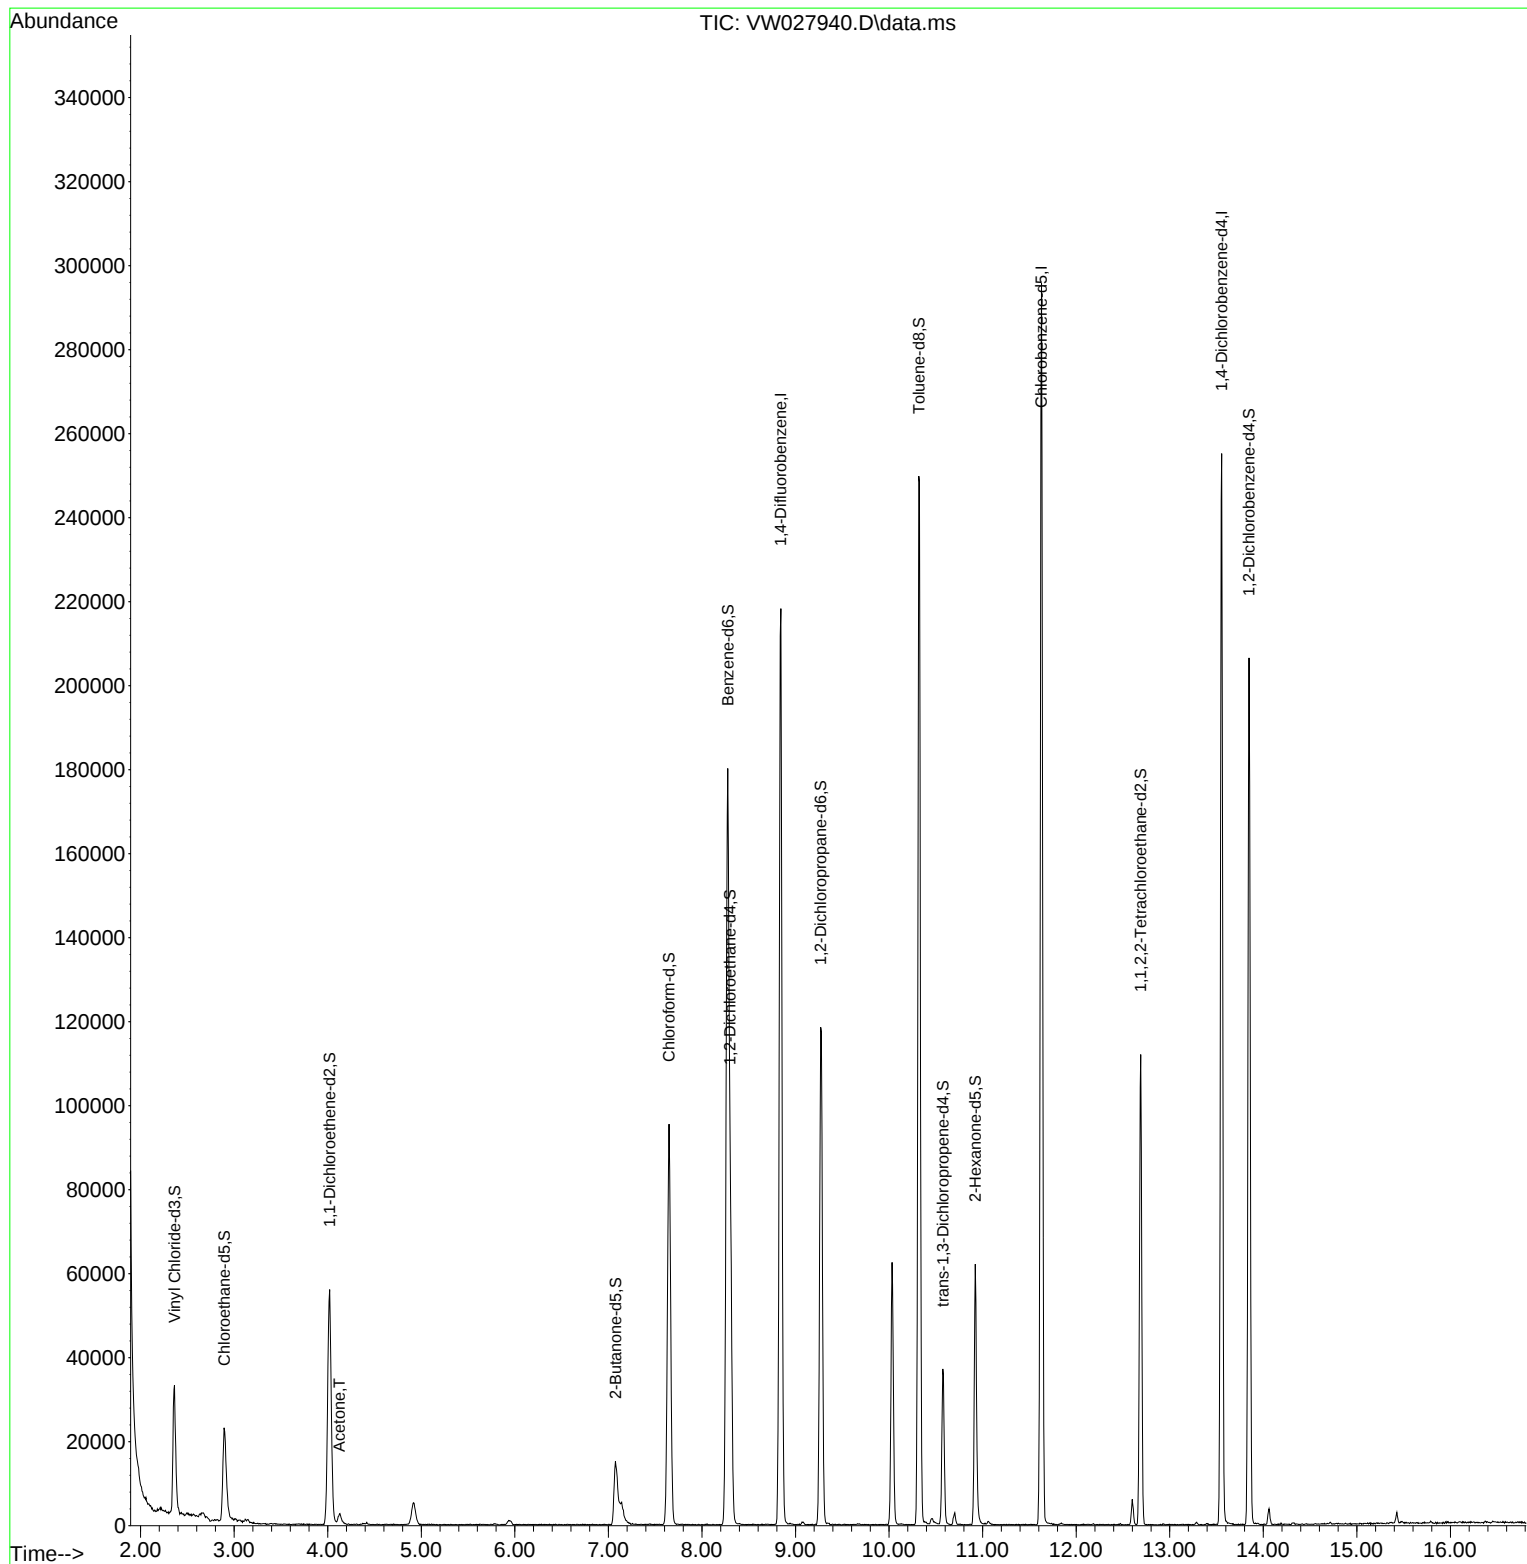

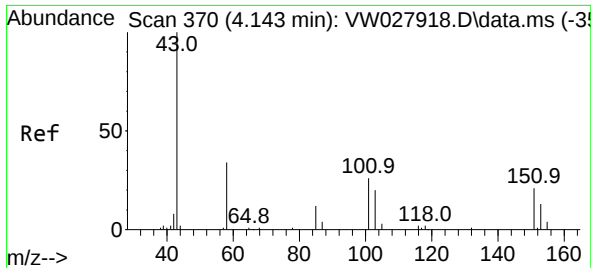

#13
 Acetone
 Concen: 8.388 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.019 min
 Lab File: VW027940.D
 Acq: 02 Feb 2024 19:19

Instrument :
 MSVOA_W
 ClientSampleId :
 BH6X5

Tgt Ion: 43 Resp: 4391
 Ion Ratio Lower Upper
 43 100
 58 37.0 0.0 70.2

