




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
Data File : VW027954.D
Acq On : 05 Feb 2024 15:20
Operator : SY/MD
Sample : P1286-09RE
Misc : 4.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH6X0

Manual IntegrationsAPPROVED

Quant Time: Feb 06 04:07:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 06 04:06:06 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

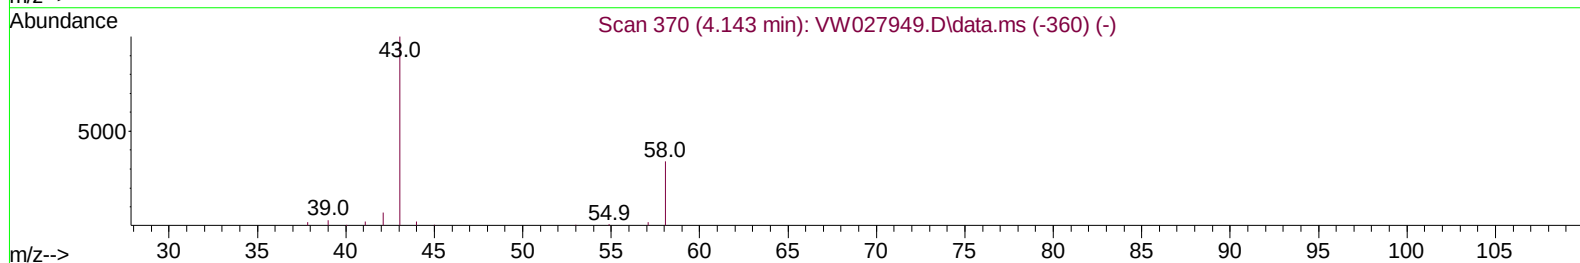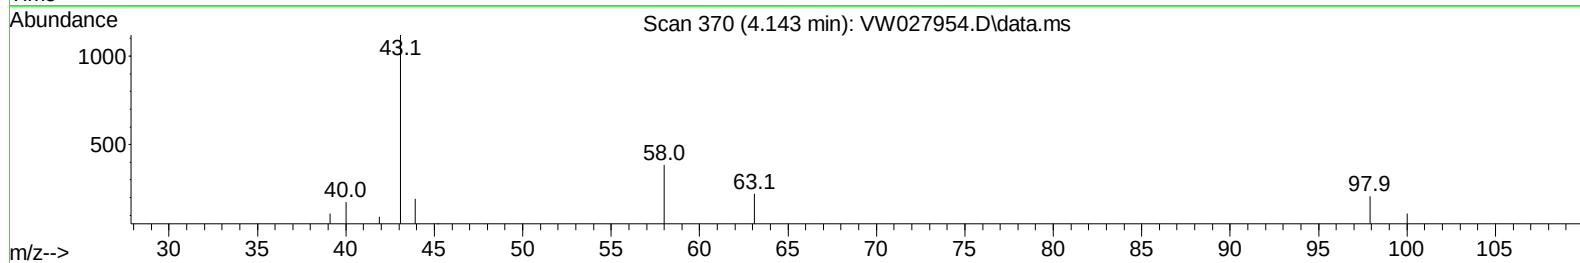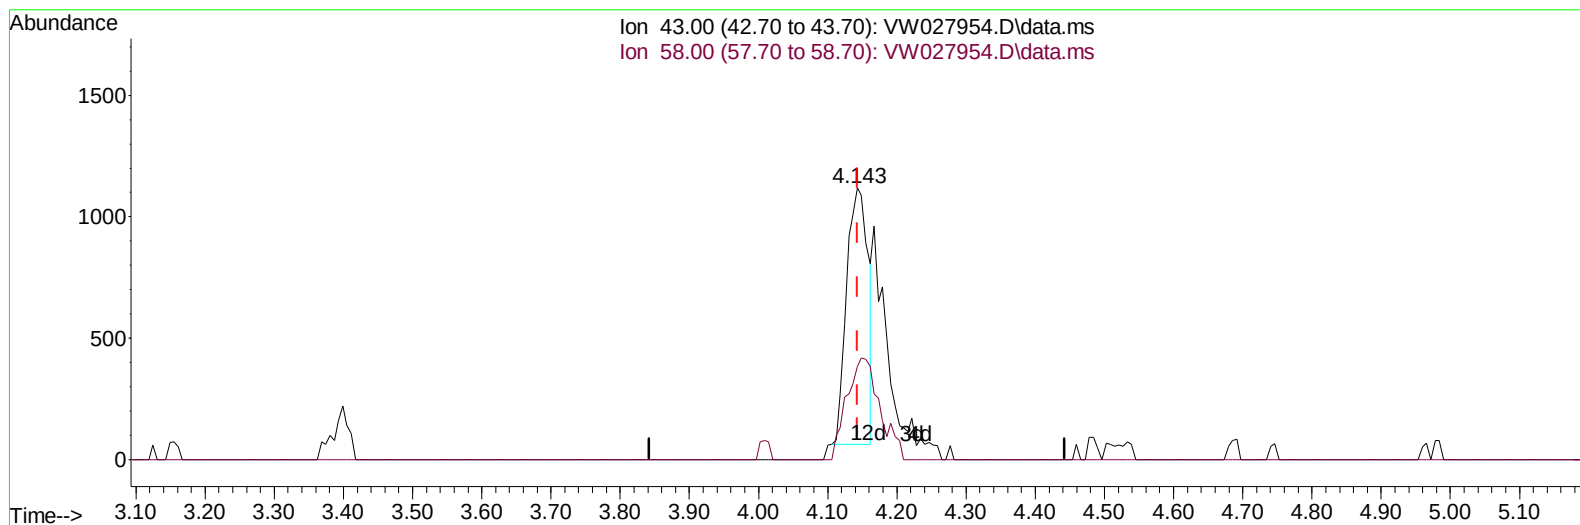

TIC: VW027954.D\data.ms

(13) Acetone (T)

4.143min (-0.000) 2.96 ug/L

response 2263

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.00	55.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
Data File : VW027954.D
Acq On : 05 Feb 2024 15:20
Operator : SY/MD
Sample : P1286-09RE
Misc : 4.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH6X0

Manual IntegrationsAPPROVED

Quant Time: Feb 06 04:07:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 06 04:06:06 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

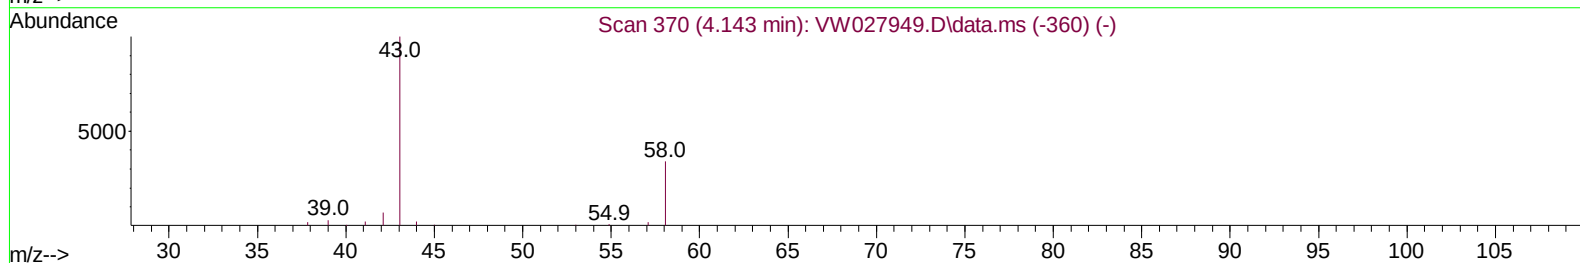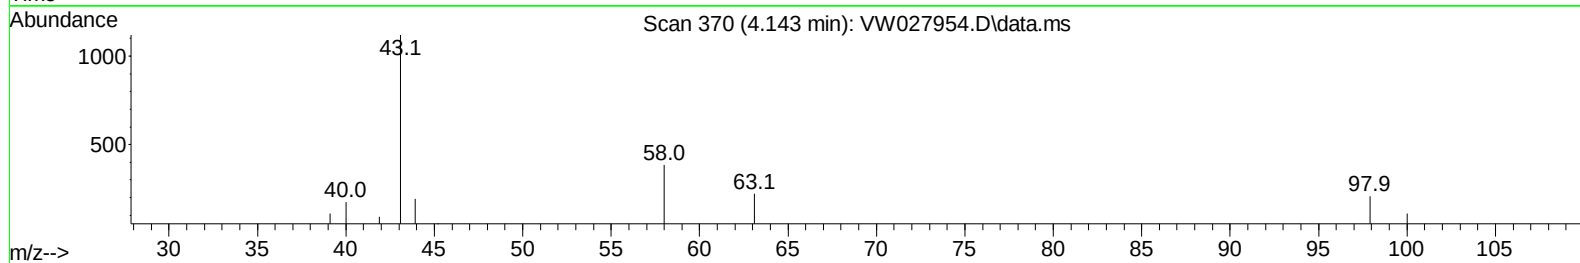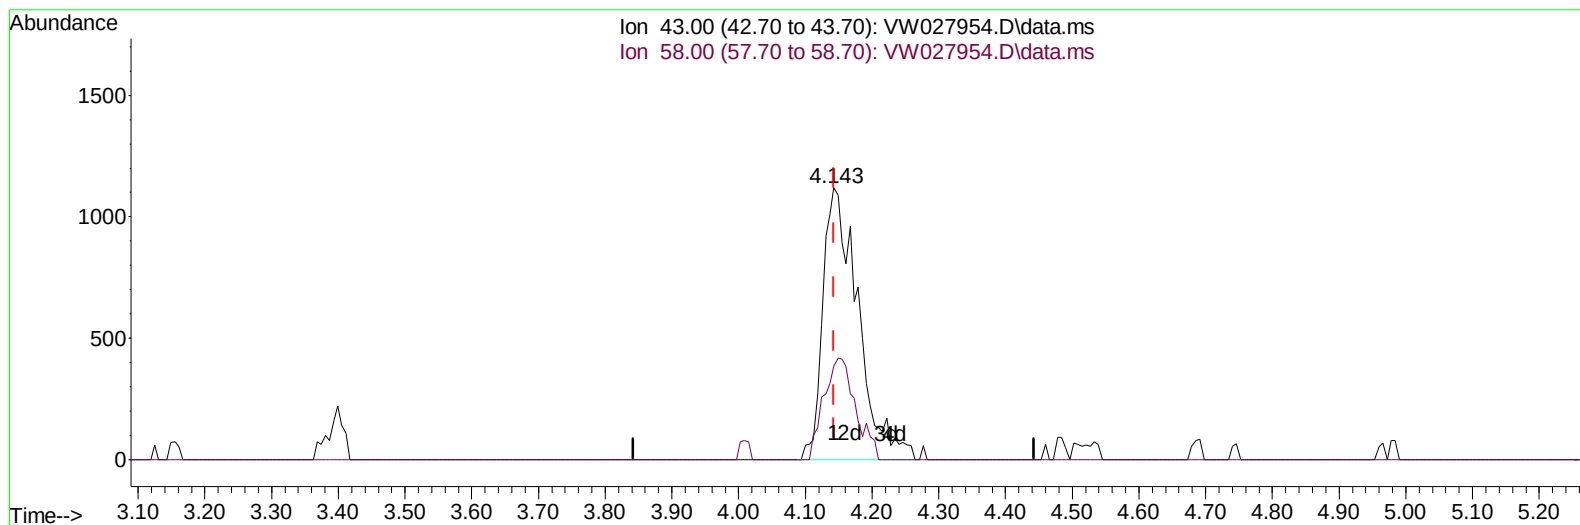

TIC: VW027954.D\data.ms

(13) Acetone (T)

4.143min (-0.000) 5.33 ug/L m

response 4082

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.00	30.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
 Data File : VW027954.D
 Acq On : 05 Feb 2024 15:20
 Operator : SY/MD
 Sample : P1286-09RE
 Misc : 4.26g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH6X0

Manual IntegrationsAPPROVED

Quant Time: Feb 06 04:07:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 06 04:06:06 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
 Supervised By :Mahesh Dadoda 02/06/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	432660	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	384886	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	166105	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	86384	17.047	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.200%	
7) Chloroethane-d5	2.899	69	72757	18.930	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.720%	
11) 1,1-Dichloroethene-d2	4.021	65	37838	17.451	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.800%	
21) 2-Butanone-d5	7.081	46	46782	59.415	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	118.840%	
24) Chloroform-d	7.648	84	204163	20.181	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	80.720%	
26) 1,2-Dichloroethane-d4	8.307	65	102977	22.538	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.160%	
32) Benzene-d6	8.276	84	421977	20.492	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.960%	
36) 1,2-Dichloropropane-d6	9.270	67	120666	21.612	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	86.440%	
41) Toluene-d8	10.325	98	387132	19.648	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	10.574	79	48500	21.123	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.480%	
47) 2-Hexanone-d5	10.922	63	45807	60.316	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.640%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	106669	25.561	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.240%	
66) 1,2-Dichlorobenzene-d4	13.848	152	130128	23.049	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.200%	
Target Compounds						
						Qvalue
13) Acetone	4.143	43	4082m	5.332	ug/L	
14) Carbon disulfide	4.393	76	8018	0.573	ug/L	96
16) Methylene chloride	4.923	84	16599	3.069	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
Data File : VW027954.D
Acq On : 05 Feb 2024 15:20
Operator : SY/MD
Sample : P1286-09RE
Misc : 4.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH6X0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 06 04:07:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 06 04:06:06 2024
Response via : Initial Calibration

