

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
 Data File : VW027951.D
 Acq On : 05 Feb 2024 14:08
 Operator : SY/MD
 Sample : P1305-08
 Misc : 5.08g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Feb 06 04:06:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 06 04:06:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	308800	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	279631	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	141740	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	91832	25.391	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.560%
7) Chloroethane-d5	2.899	69	71181	25.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.800%
11) 1,1-Dichloroethene-d2	4.021	65	37555	24.267	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	97.080%
21) 2-Butanone-d5	7.094	46	38128	67.847	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	135.700%#
24) Chloroform-d	7.648	84	183501	25.414	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.640%
26) 1,2-Dichloroethane-d4	8.307	65	91304	27.998	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.000%
32) Benzene-d6	8.276	84	395173	26.414	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.640%
36) 1,2-Dichloropropane-d6	9.270	67	105078	25.904	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.600%
41) Toluene-d8	10.319	98	369494	25.812	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.240%
43) trans-1,3-Dichloroprop...	10.575	79	45192	27.090	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	108.360%
47) 2-Hexanone-d5	10.922	63	37092	67.224	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.440%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91124	30.055	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.240%#
66) 1,2-Dichlorobenzene-d4	13.849	152	133313	27.672	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.680%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	8452	2.190	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
Data File : VW027951.D
Acq On : 05 Feb 2024 14:08
Operator : SY/MD
Sample : P1305-08
Misc : 5.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Feb 06 04:06:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 06 04:06:06 2024
Response via : Initial Calibration

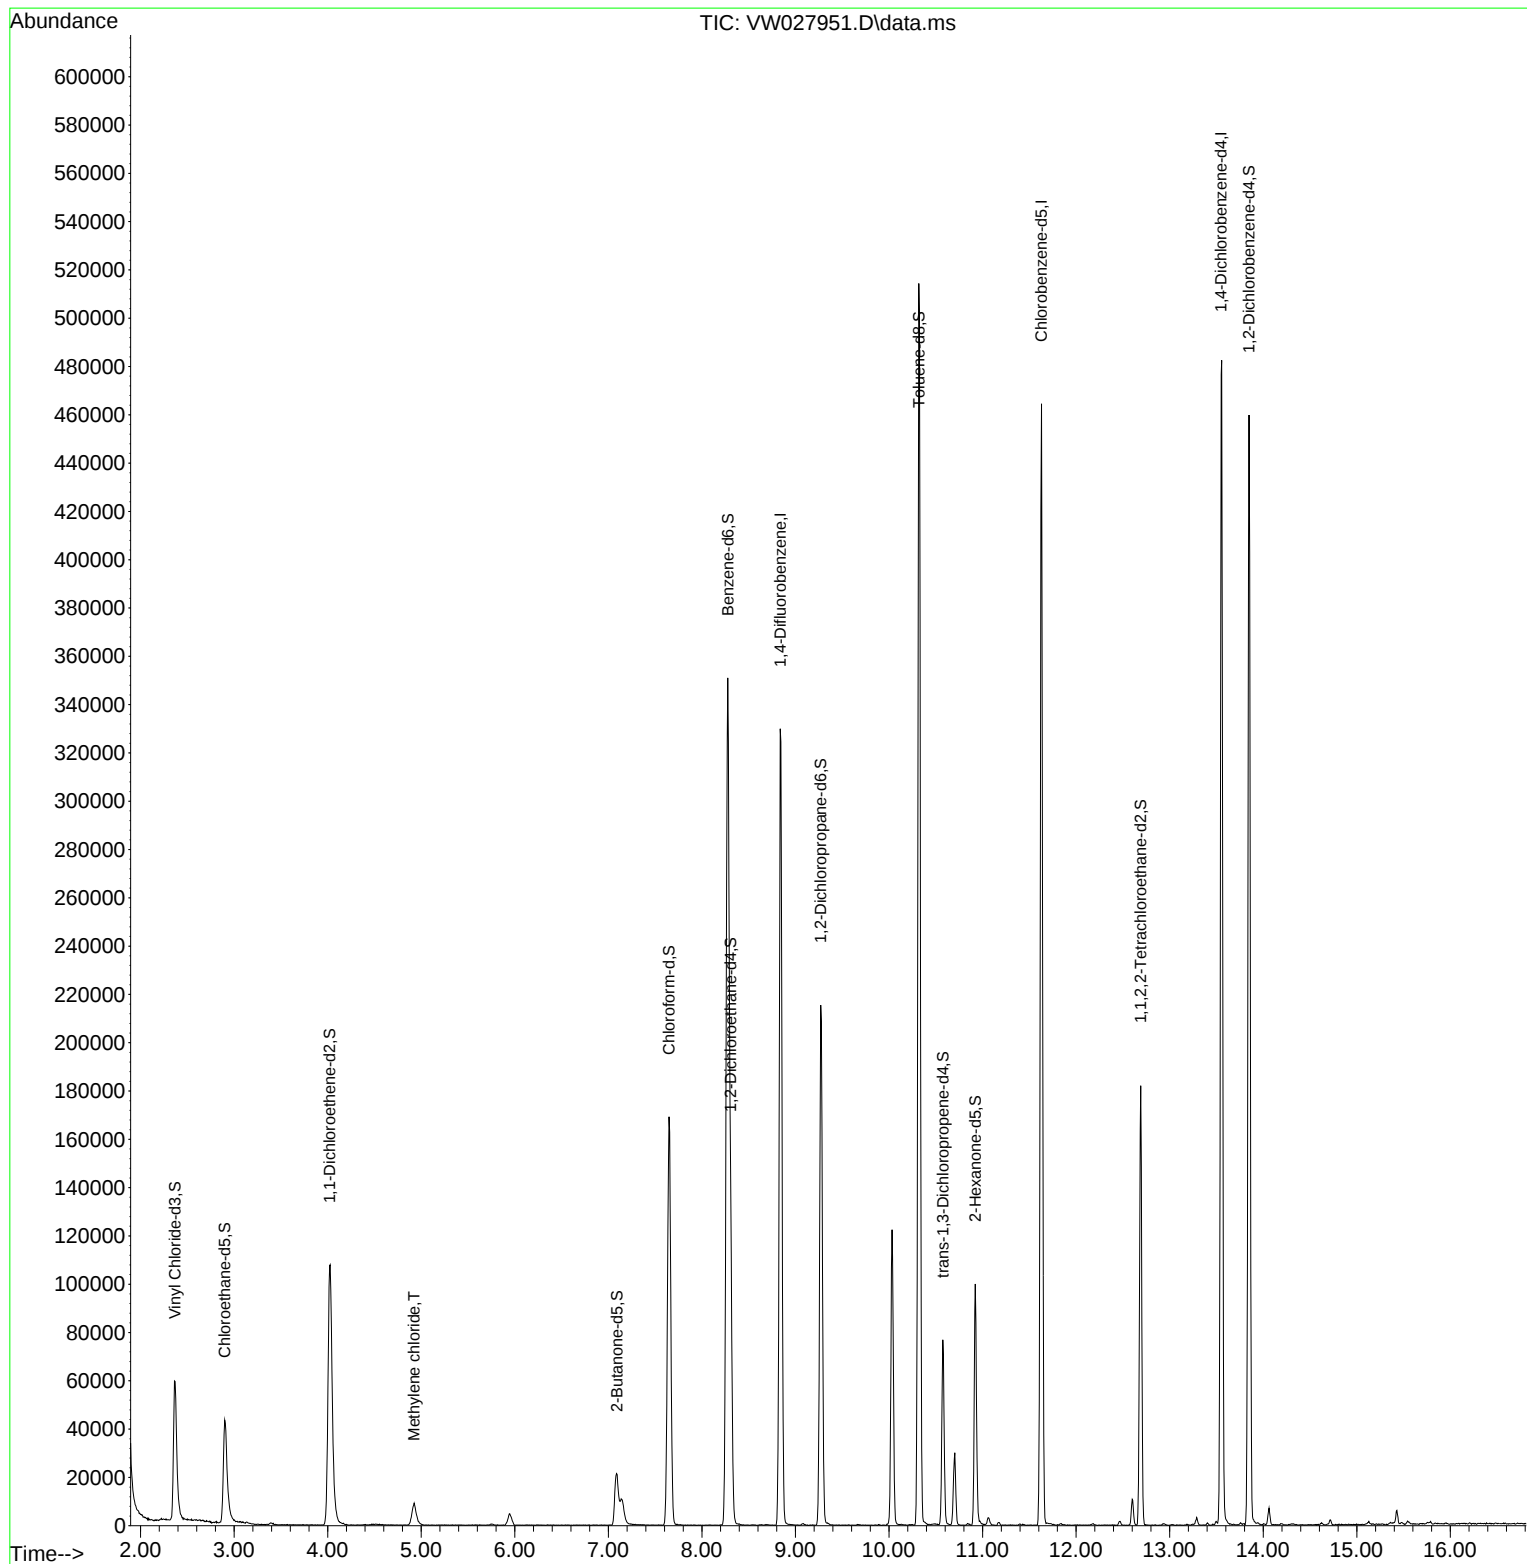

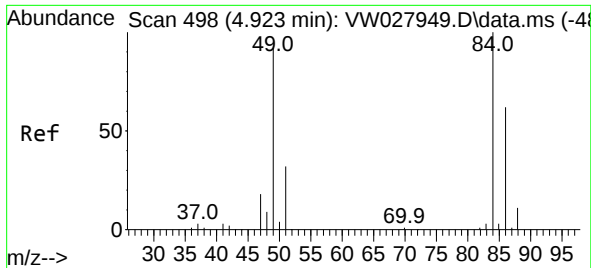

#16
Methylene chloride
Concen: 2.190 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW027951.D
Acq: 05 Feb 2024 14:08

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

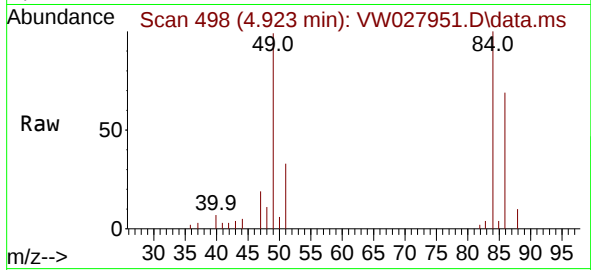

Tgt Ion: 84 Resp: 8452

Ion	Ratio	Lower	Upper
84	100		
86	69.3	45.4	84.4
49	98.6	66.3	123.1

