

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
 Data File : VW027955.D
 Acq On : 05 Feb 2024 15:43
 Operator : SY/MD
 Sample : P1286-10
 Misc : 5.46g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH6X1

Quant Time: Feb 06 04:07:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 06 04:06:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	399709	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.623	117	357258	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	161666	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	85211	18.202	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.800%		
7) Chloroethane-d5	2.899	69	75069	21.141	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.560%		
11) 1,1-Dichloroethene-d2	4.021	65	37307	18.624	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.480%		
21) 2-Butanone-d5	7.088	46	48425	66.572	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	133.140%		
24) Chloroform-d	7.648	84	205035	21.938	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.760%		
26) 1,2-Dichloroethane-d4	8.307	65	104661	24.795	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.160%		
32) Benzene-d6	8.276	84	426680	22.323	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.280%		
36) 1,2-Dichloropropane-d6	9.270	67	120631	23.276	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.120%		
41) Toluene-d8	10.319	98	385908	21.101	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.400%		
43) trans-1,3-Dichloroprop...	10.575	79	50408	23.651	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	94.600%		
47) 2-Hexanone-d5	10.922	63	48028	68.131	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	136.260%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	107158	27.664	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	110.640%		
66) 1,2-Dichlorobenzene-d4	13.849	152	132209	24.060	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.240%		
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	15381	3.079	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020524\
Data File : VW027955.D
Acq On : 05 Feb 2024 15:43
Operator : SY/MD
Sample : P1286-10
Misc : 5.46g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH6X1

Quant Time: Feb 06 04:07:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 06 04:06:06 2024
Response via : Initial Calibration

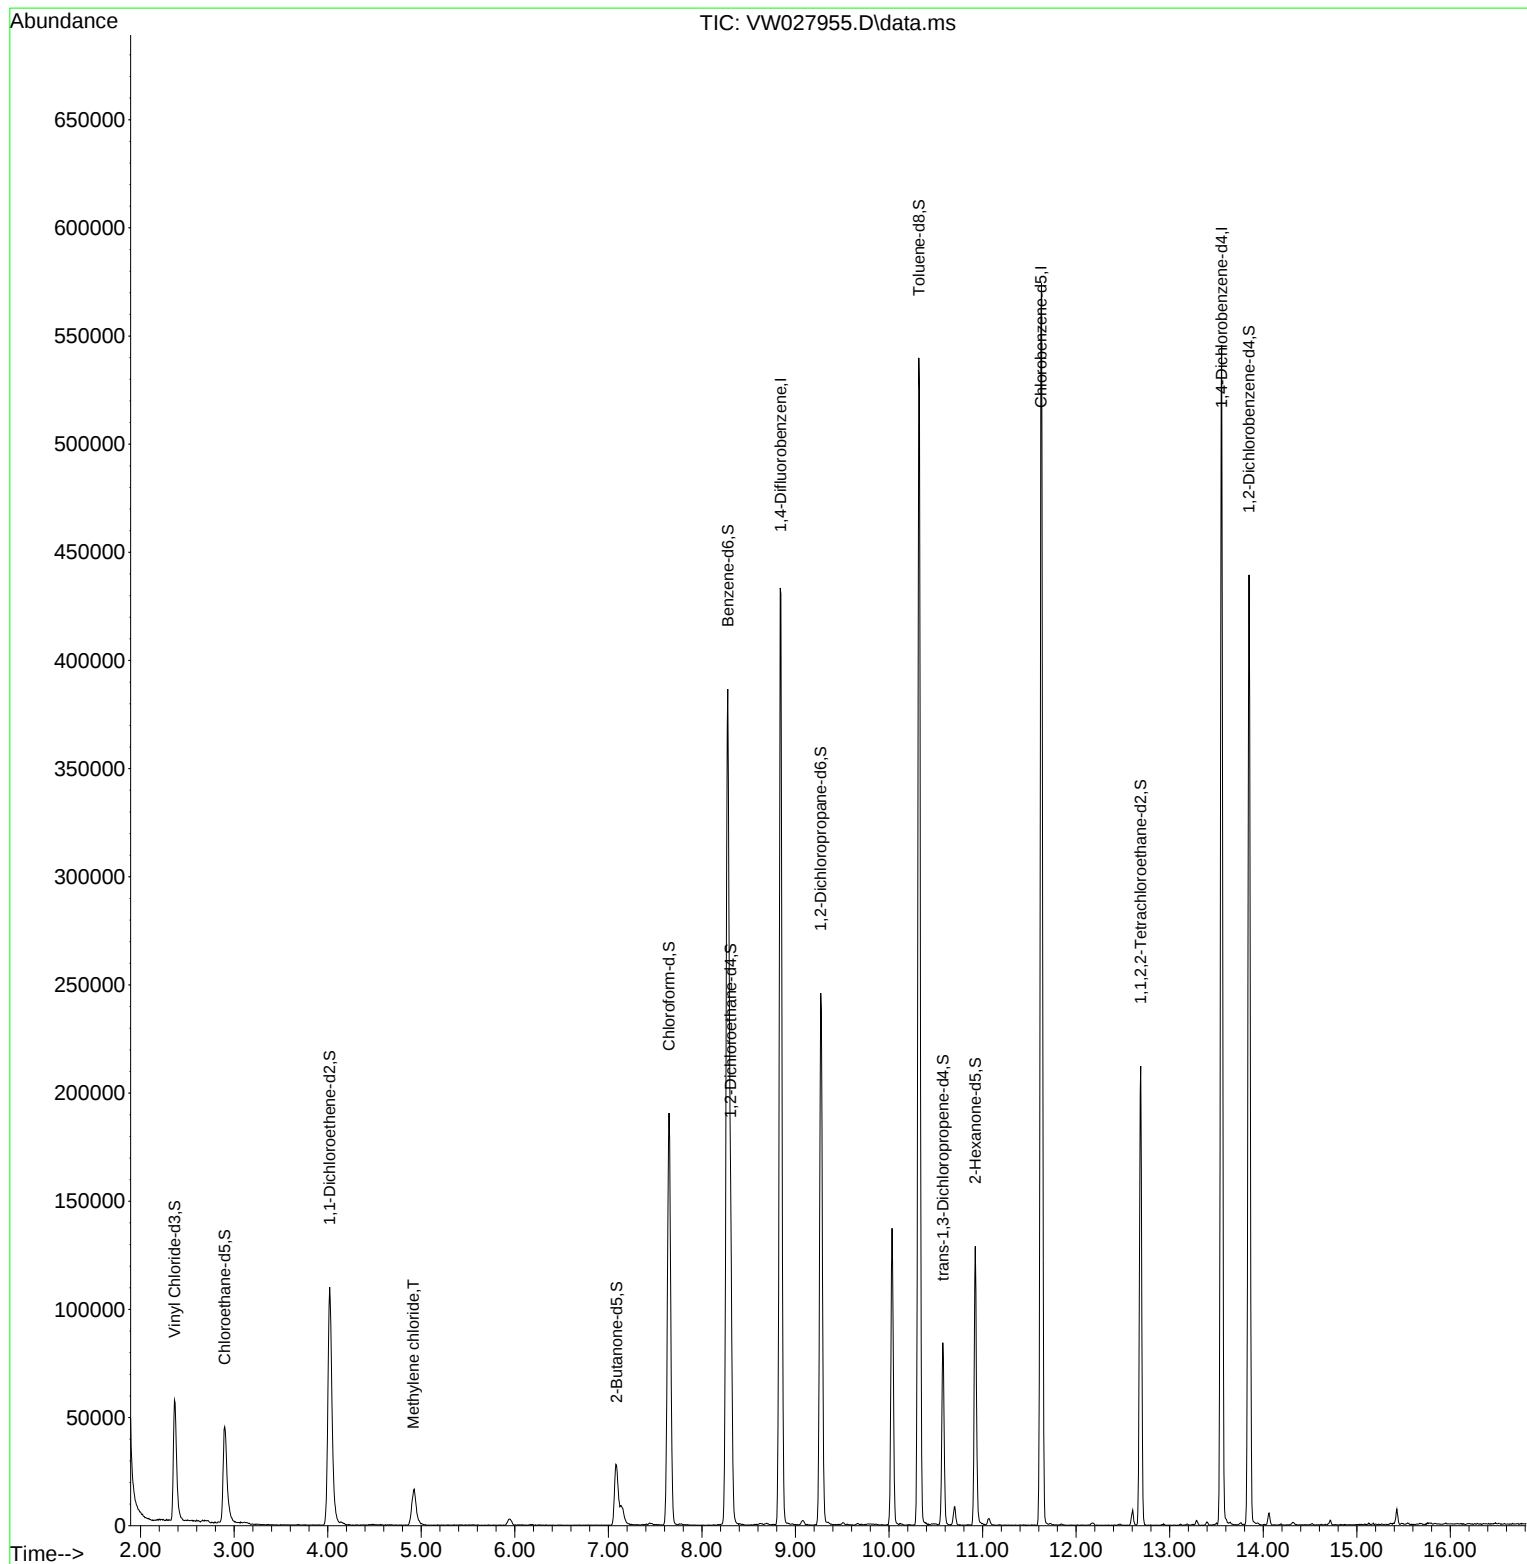

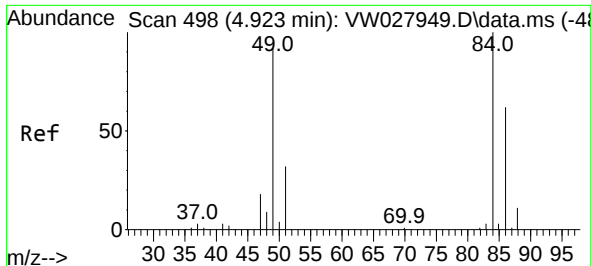

#16
Methylene chloride
Concen: 3.079 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW027955.D
Acq: 05 Feb 2024 15:43

Instrument :
MSVOA_W
ClientSampleId :
BH6X1

Tgt Ion: 84 Resp: 15381
Ion Ratio Lower Upper
84 100
86 58.5 45.4 84.4
49 95.9 66.3 123.1

