

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020623\
 Data File : VW025288.D
 Acq On : 06 Feb 2023 10:14
 Operator : SY/MD
 Sample : VW0206SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK459

Quant Time: Feb 07 00:19:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 07 00:17:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	371357	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	336576	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	119546	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.367	65	90840	25.278	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.120%
7) Chloroethane-d5	2.903	69	79072	24.781	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.120%
11) 1,1-Dichloroethene-d2	4.019	63	175616	17.624	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.480%
21) 2-Butanone-d5	7.079	46	50892	54.553	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.100%
24) Chloroform-d	7.652	84	238913	24.546	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	8.305	65	126925	26.771	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.080%
32) Benzene-d6	8.274	84	481623	23.610	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.440%
36) 1,2-Dichloropropane-d6	9.274	67	139931	23.444	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.760%
41) Toluene-d8	10.323	98	434290	23.817	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.280%
43) trans-1,3-Dichloroprop...	10.579	79	57803	25.918	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	103.680%
47) 2-Hexanone-d5	10.920	63	40117	59.947	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.900%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	72097	17.763	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	71.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	108248	26.099	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.400%
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	9.268	63	16159	2.813	ug/L	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020623\
Data File : VW025288.D
Acq On : 06 Feb 2023 10:14
Operator : SY/MD
Sample : VW0206SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK459

Quant Time: Feb 07 00:19:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 07 00:17:55 2023
Response via : Initial Calibration

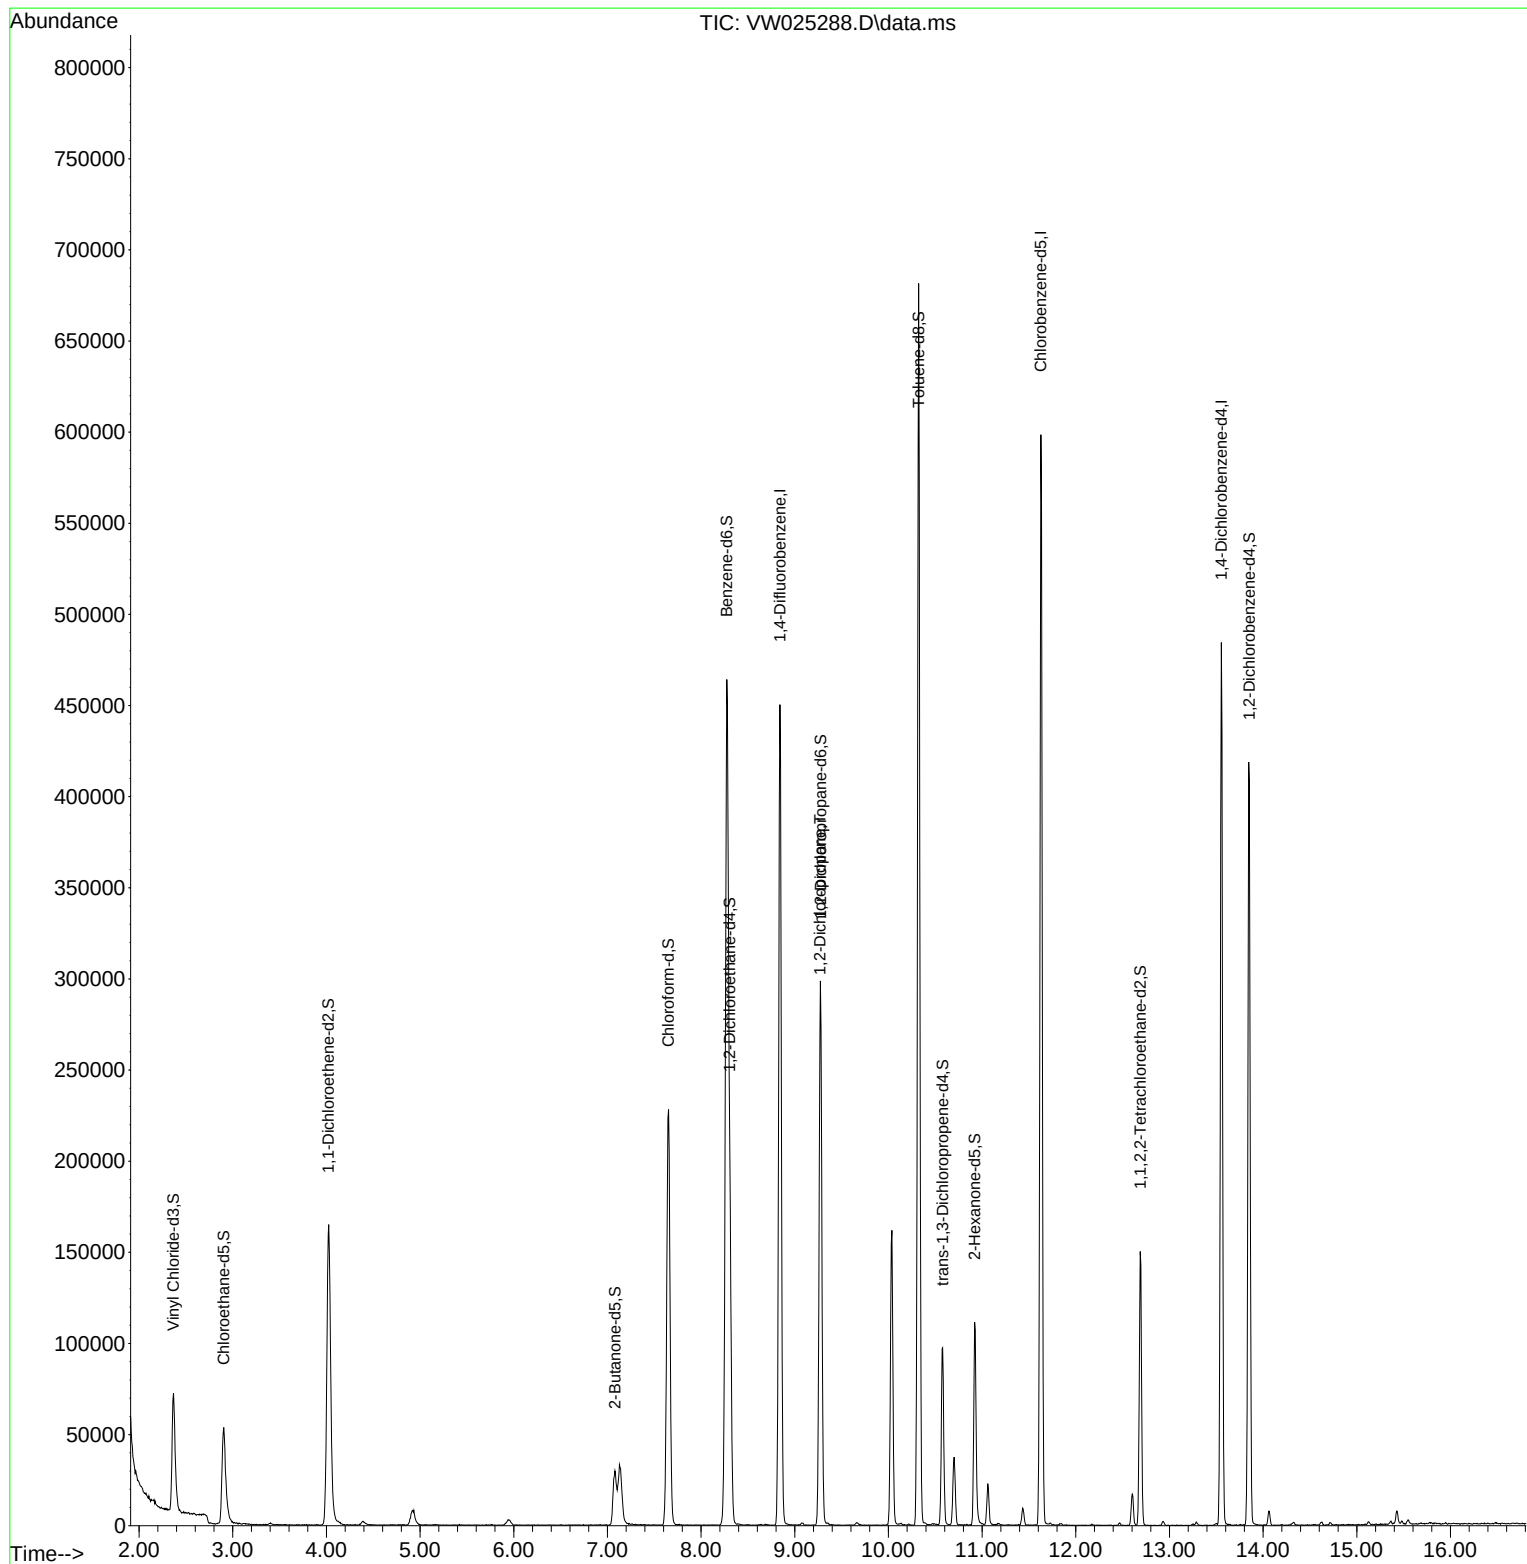

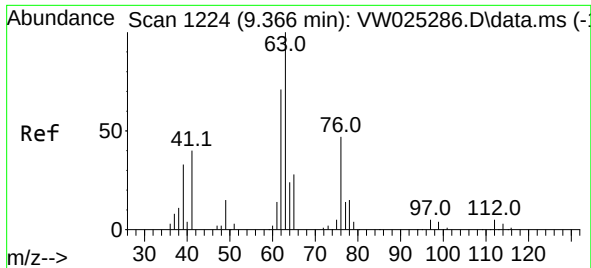

#37

1,2-Dichloropropane

Concen: 2.813 ug/L

RT: 9.268 min Scan# 11

Delta R.T. -0.098 min

Lab File: VW025288.D

Acq: 06 Feb 2023 10:14

Instrument :

MSVOA_W

ClientSampleId :

VBLK459

Tgt Ion: 63 Resp: 16159

Ion Ratio Lower Upper

63 100

112 0.2 3.8 5.8#

