
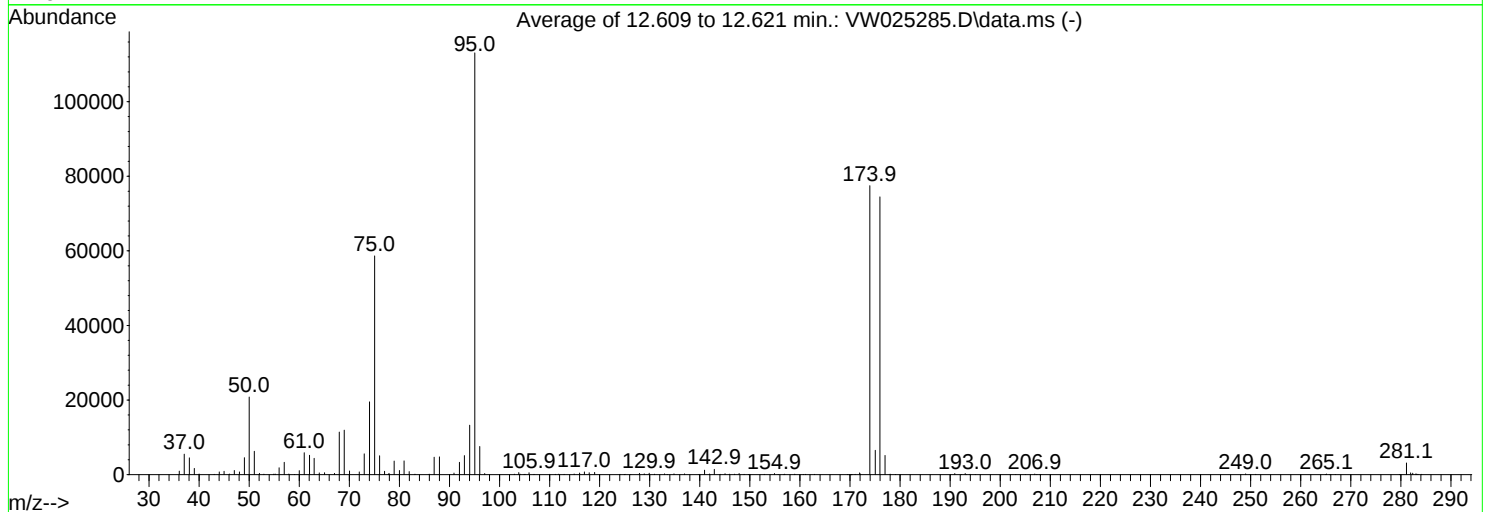


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020623\
Data File : VW025285.D
Acq On : 06 Feb 2023 07:27
Operator : SY/MD
Sample : BFB476
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB476

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Title : SFAM01.0
Last Update : Tue Feb 07 00:17:55 2023

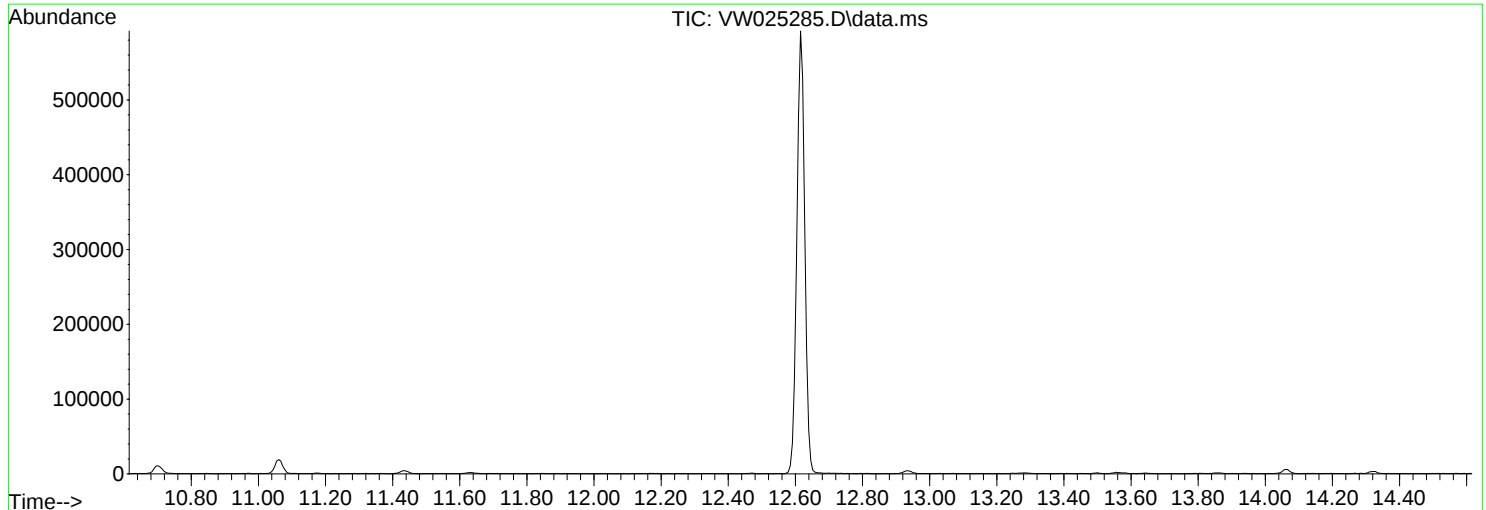

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	20805	PASS
75	95	30	80	51.9	58669	PASS
95	95	100	100	100.0	113099	PASS
96	95	5	9	6.7	7552	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.5	77499	PASS
175	174	5	9	8.4	6542	PASS
176	174	95	105	96.1	74499	PASS
177	176	5	10	6.9	5150	PASS

m/z	Abundance
40.00	93.0
44.20	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

m/z	Abundance
36.10	890.0
37.10	5200.0
38.00	4165.0
39.00	1589.0
40.10	299.0
43.00	76.0
44.00	948.0
45.00	944.0
46.00	194.0
47.00	1000.0
48.10	648.0
49.00	4232.0
50.00	19272.0
51.10	5964.0
52.10	352.0
53.00	113.0
55.00	219.0
56.00	1634.0
57.00	3086.0
58.00	204.0
59.10	80.0
60.10	786.0
61.00	5582.0
62.00	4871.0
63.00	4327.0
64.00	376.0
65.00	536.0
67.00	358.0
68.00	10797.0
69.00	10826.0
70.10	832.0
72.00	665.0
73.00	5402.0
74.00	17896.0
75.00	54328.0
76.00	4857.0
77.10	716.0
77.80	453.0
79.00	3427.0
80.10	1020.0
80.90	3442.0
82.00	675.0
83.10	93.0
86.10	68.0
87.00	4360.0
88.00	4695.0
90.90	391.0
92.00	3223.0
93.00	4378.0
94.10	11314.0
95.00	101992.0
96.00	6965.0
97.10	317.0
103.00	132.0
103.80	351.0
104.10	368.0
104.90	99.0
105.90	449.0
106.90	153.0
110.10	161.0
111.20	66.0
111.90	98.0
114.90	158.0
116.10	381.0
116.90	579.0
117.90	503.0
119.00	539.0
124.90	185.0
126.20	139.0
128.00	282.0
129.00	210.0
129.90	290.0
131.00	66.0
132.90	267.0
134.90	184.0
136.90	197.0
139.80	103.0
141.00	1183.0
142.00	165.0
142.90	1092.0
144.10	89.0
145.10	181.0
145.90	130.0
147.00	146.0
147.90	278.0
148.80	83.0
150.00	104.0
152.80	146.0
155.00	221.0
156.80	93.0
159.00	79.0
160.70	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

161.20	53.0
162.90	181.0
169.50	60.0
169.80	59.0
171.90	704.0
174.00	64368.0
175.00	4956.0
176.00	60504.0
177.00	4528.0
178.00	225.0
179.10	90.0
191.00	319.0
192.20	87.0
193.00	465.0
193.90	166.0
195.00	77.0
203.10	94.0
205.00	62.0
206.90	326.0
207.90	53.0
249.00	234.0
249.90	94.0
251.00	149.0
265.20	362.0
266.90	124.0
279.70	60.0
281.00	4184.0
282.00	1108.0
283.00	630.0
284.20	141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

m/z	Abundance
36.10	953.0
37.00	5917.0
38.10	5141.0
39.10	2153.0
40.00	236.0
43.00	91.0
44.10	855.0
45.00	908.0
46.10	114.0
47.10	1306.0
48.00	918.0
49.10	5154.0
50.00	23328.0
51.10	7002.0
52.10	397.0
52.90	99.0
54.80	233.0
55.20	344.0
56.00	2241.0
57.00	3667.0
58.00	188.0
60.00	1325.0
61.00	6522.0
62.10	5684.0
63.00	4560.0
64.00	502.0
65.00	566.0
67.00	356.0
68.00	12903.0
69.00	12927.0
70.10	1222.0
72.10	909.0
73.00	5810.0
74.00	22488.0
75.10	66184.0
76.10	5506.0
77.00	1204.0
78.00	470.0
78.90	4025.0
79.90	1140.0
81.00	4176.0
82.00	958.0
82.90	115.0
83.20	105.0
86.00	119.0
86.90	5110.0
88.00	5142.0
91.00	507.0
92.00	3626.0
93.00	5833.0
94.00	14444.0
95.10	126920.0
96.10	8377.0
97.00	308.0
102.90	176.0
103.80	576.0
105.10	239.0
105.90	539.0
106.90	95.0
110.00	90.0
111.20	89.0
111.80	100.0
112.90	121.0
114.90	217.0
115.90	357.0
117.00	840.0
118.00	442.0
119.00	672.0
124.00	115.0
125.10	161.0
127.80	313.0
128.80	220.0
129.80	427.0
130.90	160.0
133.00	199.0
134.80	269.0
137.00	181.0
139.90	144.0
140.90	1293.0
141.90	173.0
142.90	1742.0
143.90	114.0
145.00	450.0
145.90	150.0
146.90	141.0
147.80	339.0
148.80	94.0
149.70	117.0
152.90	153.0
155.00	294.0
155.60	105.0
157.00	203.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

158.90	184.0
160.70	91.0
161.20	125.0
162.90	92.0
169.50	82.0
170.00	88.0
171.10	164.0
171.90	706.0
173.90	82328.0
175.00	7340.0
176.00	85064.0
177.00	5140.0
178.10	115.0
179.00	97.0
190.80	428.0
192.20	71.0
193.00	431.0
194.00	57.0
195.00	75.0
203.10	72.0
205.00	101.0
206.80	122.0
207.30	140.0
249.00	248.0
251.00	108.0
265.00	203.0
265.80	67.0
279.70	56.0
281.10	3612.0
282.30	829.0
283.20	386.0
284.10	107.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

m/z	Abundance
36.00	974.0
37.10	5323.0
38.00	4269.0
39.00	1343.0
40.00	235.0
43.00	105.0
44.10	810.0
45.00	840.0
46.10	159.0
47.10	1005.0
48.10	607.0
49.00	4268.0
50.00	19816.0
51.00	5880.0
52.00	279.0
53.00	182.0
55.20	235.0
56.00	1655.0
57.00	3158.0
57.90	136.0
59.90	1116.0
61.00	5479.0
62.00	5066.0
63.00	4280.0
64.00	499.0
65.10	409.0
67.10	382.0
68.00	10605.0
69.00	12093.0
70.00	876.0
71.90	661.0
73.00	5512.0
74.10	18208.0
75.10	55496.0
76.00	4854.0
77.00	754.0
77.90	520.0
78.90	3444.0
80.00	1194.0
80.90	3452.0
81.90	835.0
83.20	94.0
85.90	200.0
87.00	4552.0
88.00	4479.0
90.80	422.0
92.00	3038.0
93.00	5074.0
94.00	14060.0
95.10	110384.0
96.10	7313.0
97.00	295.0
103.00	102.0
103.90	707.0
104.90	128.0
105.90	571.0
106.80	70.0
109.90	56.0
111.10	112.0
111.80	142.0
112.90	97.0
114.90	112.0
116.00	539.0
116.90	846.0
117.80	560.0
119.00	627.0
124.10	97.0
125.00	60.0
128.00	407.0
128.90	167.0
130.00	458.0
130.90	172.0
133.00	169.0
133.50	81.0
134.90	228.0
136.90	240.0
141.00	1120.0
141.90	155.0
142.90	1461.0
144.10	71.0
145.10	173.0
145.90	169.0
146.90	108.0
147.80	281.0
148.90	80.0
150.00	218.0
154.80	340.0
155.70	67.0
156.90	226.0
158.90	163.0
161.00	114.0
170.20	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

170.90	112.0
172.10	545.0
174.00	85800.0
175.10	7329.0
175.90	77928.0
177.00	5782.0
177.90	102.0
191.00	128.0
193.20	138.0
207.00	132.0
249.00	138.0
264.90	138.0
281.20	1564.0
281.90	375.0
282.40	300.0
283.40	219.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476