

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (QT Reviewed)


Data File : VW014923.D
Acq On : 07 Feb 2020 16:30
Operator : SY/VA
Sample : L1415-04
Misc : 5.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:42:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
F3S23

Manual Integrations
APPROVED

apatel
2/17/2020 8:51:59 AM

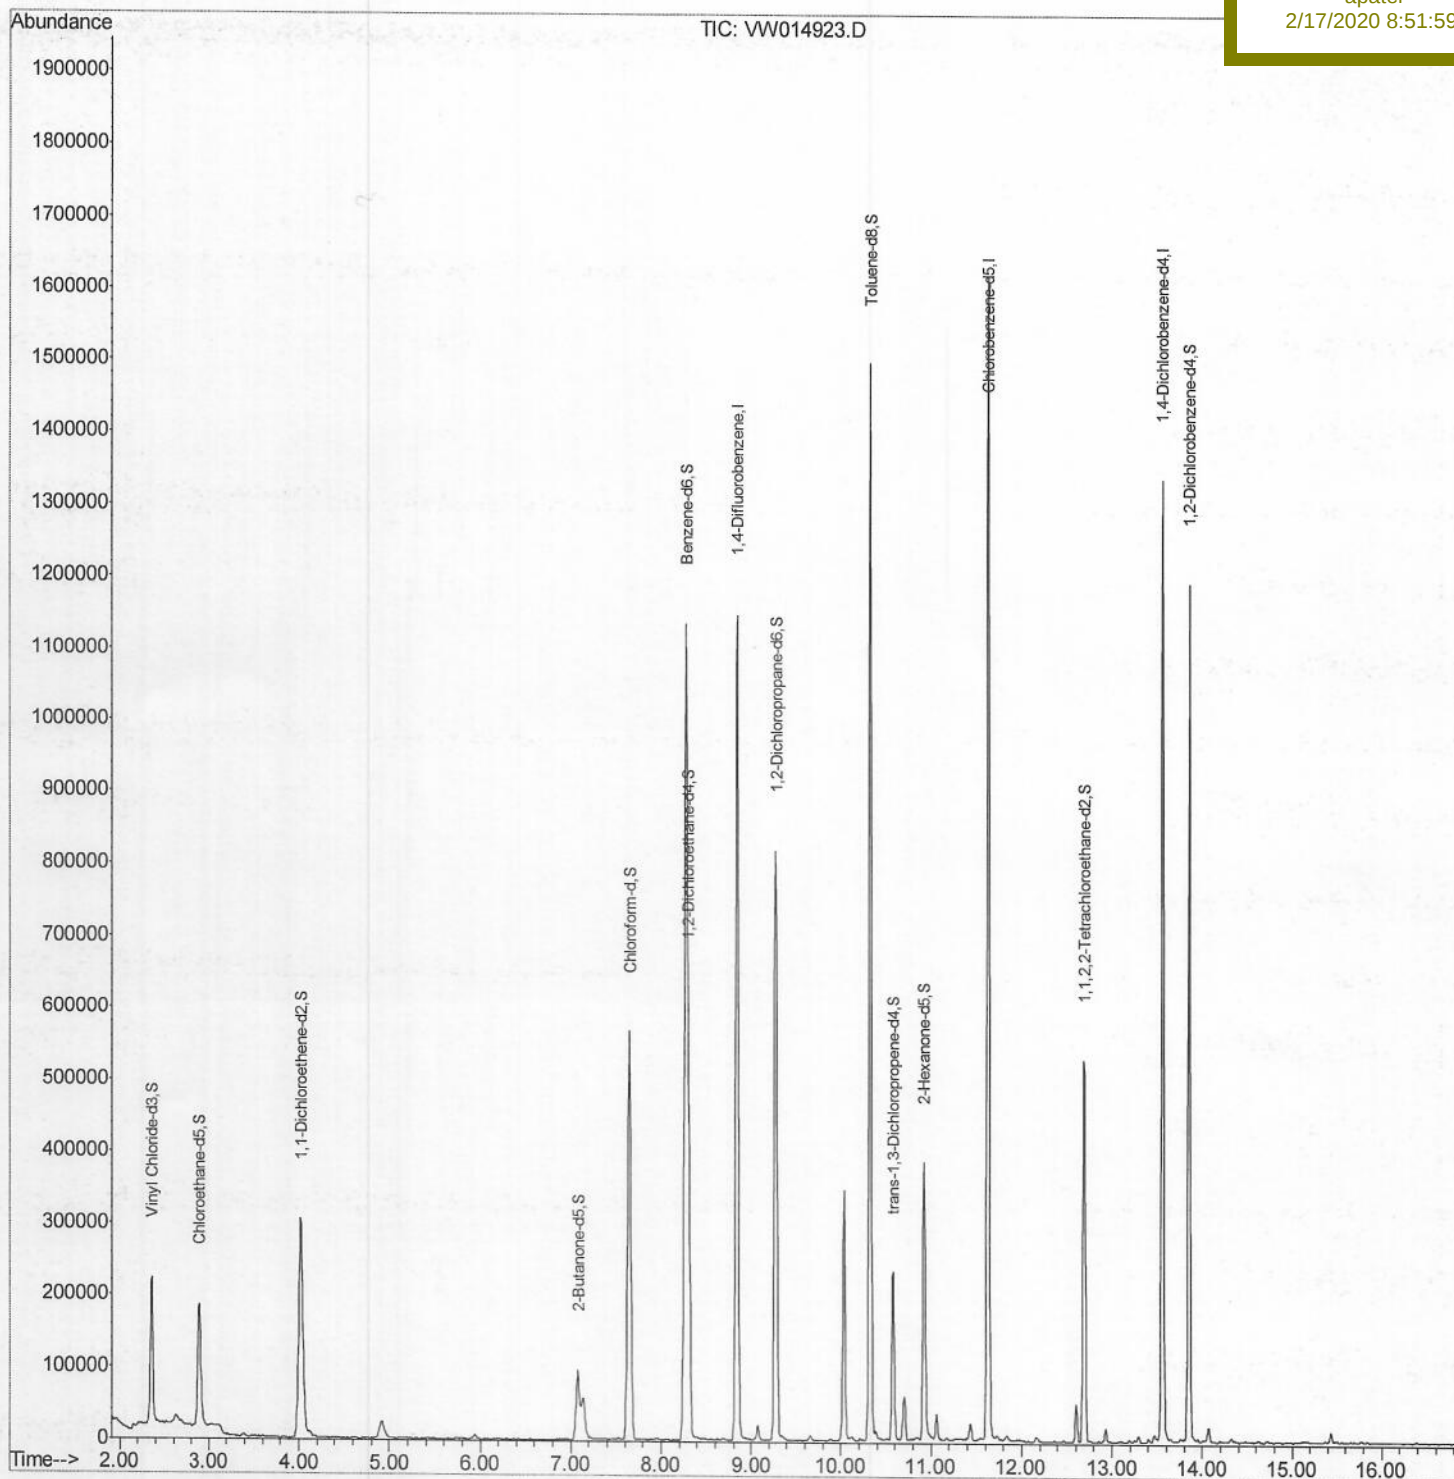

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (Qedit)




Data File : VW014923.D
Acq On : 07 Feb 2020 16:30
Operator : SY/VA
Sample : L1415-04
Misc : 5.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 04:03:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
F3S23

Manual Integrations
APPROVED

apatel
2/17/2020 8:51:59 AM

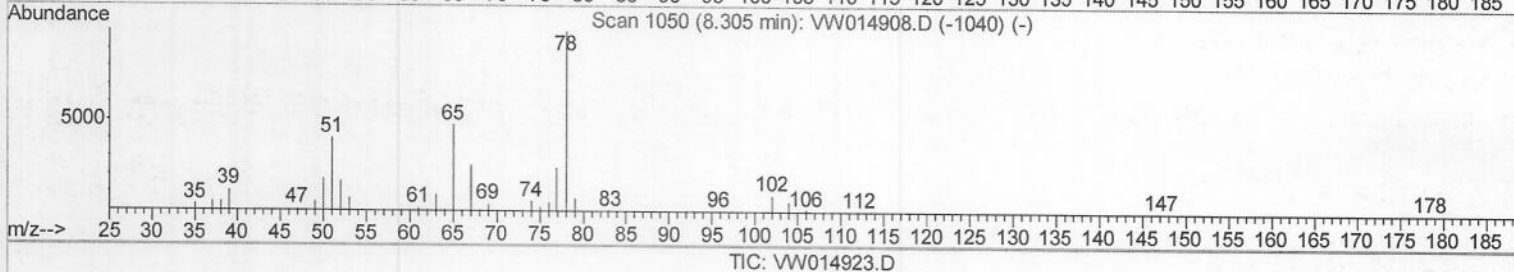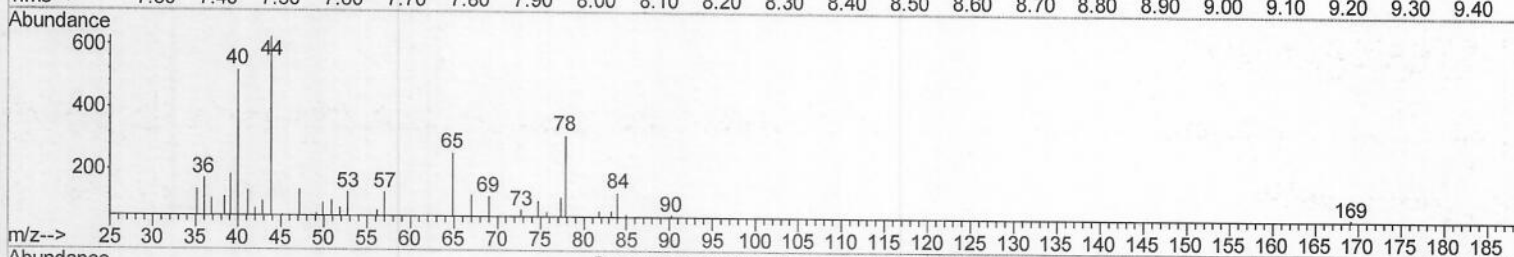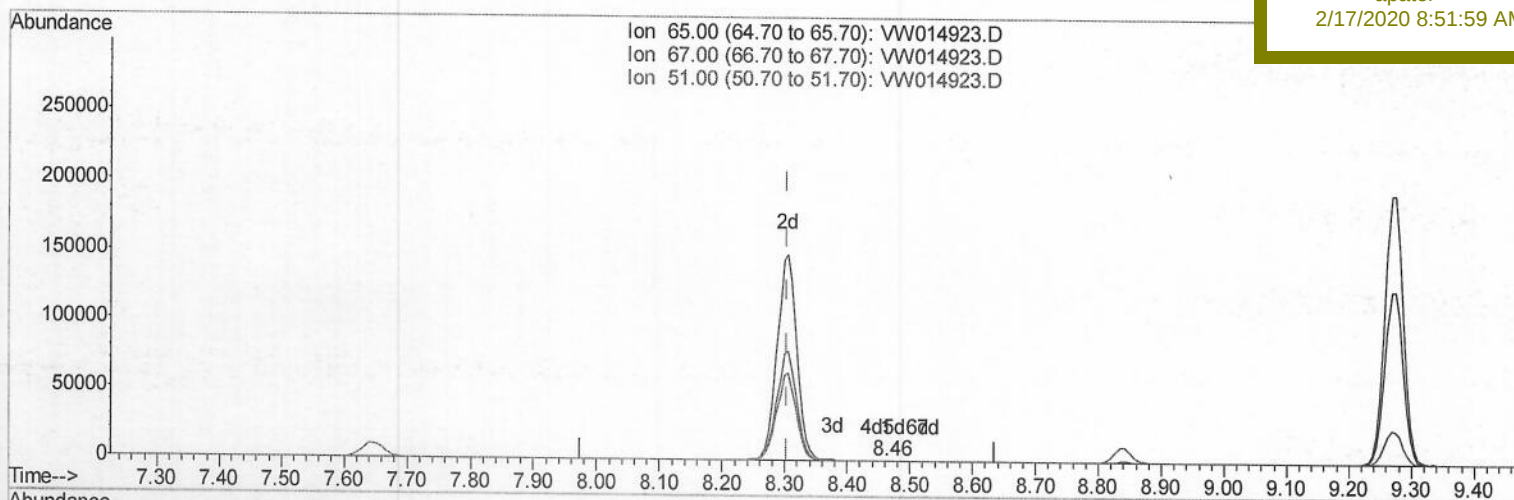

(26) 1,2-Dichloroethane-d4 (S)

8.463min (+0.158) 0.01ug/L

response 147

Ion	Exp%	Act%
65.00	100	100
67.00	53.80	49.66
51.00	115.00	141.50
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (Qedit)

Data File : VW014923.D

Acq On : 07 Feb 2020 16:30

Operator : SY/VA

Sample : L1415-04

Misc : 5.92G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 04:03:26 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M

Quant Title : VOC Analysis

QLast Update : Sat Feb 08 03:59:50 2020

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :




F3S23

Manual Integrations

APPROVED

apatel

2/17/2020 8:51:59 AM

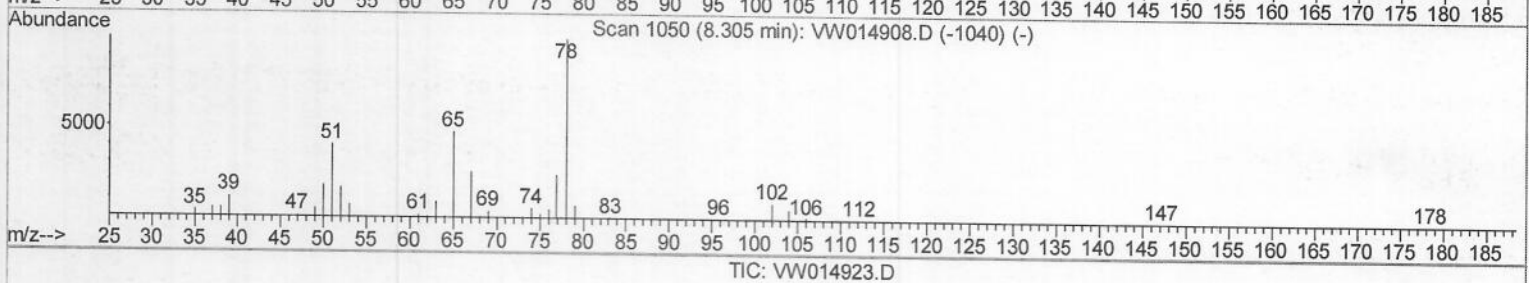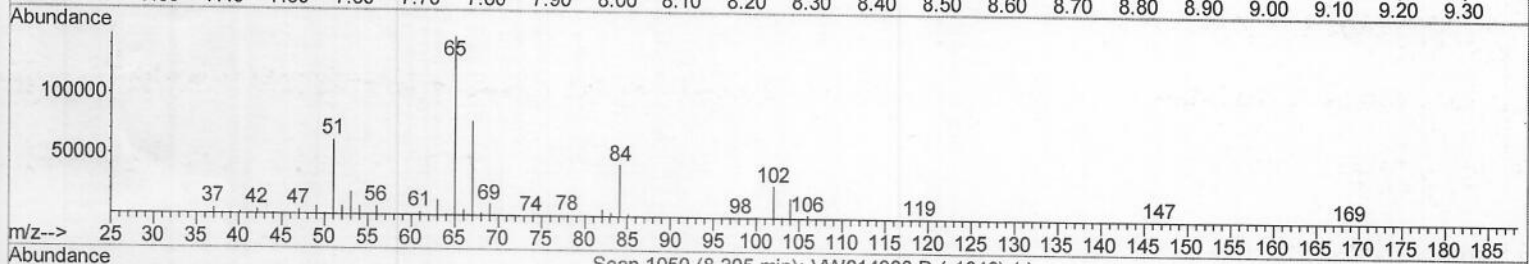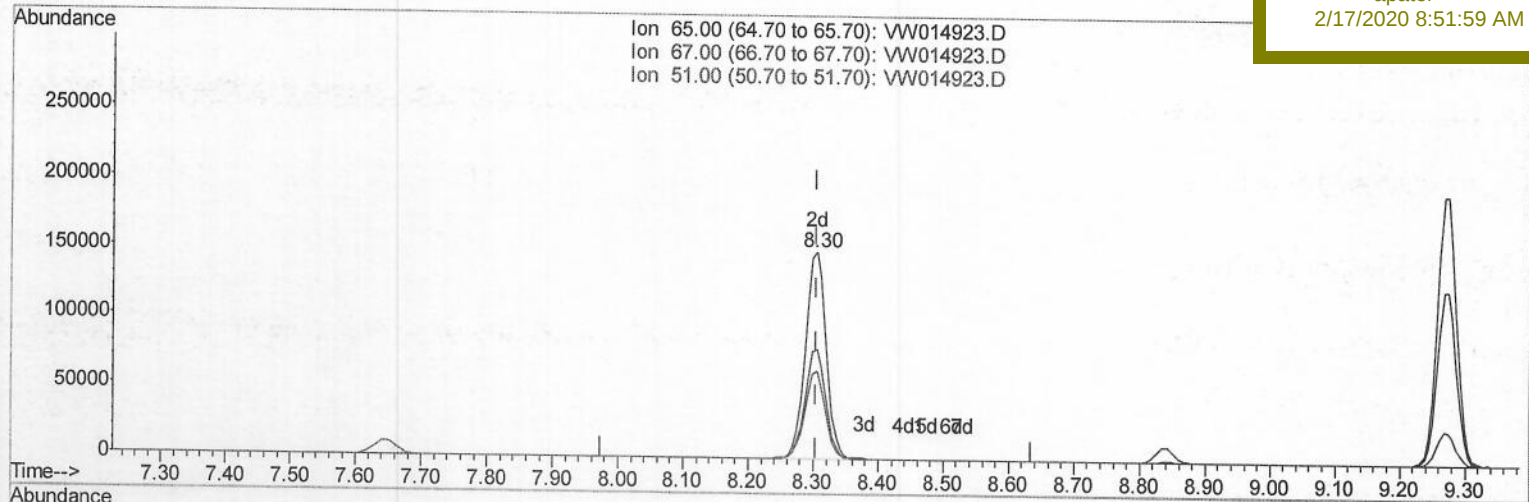

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 23.92ug/L m

response 325729

Ion	Exp%	Act%
65.00	100	100
67.00	53.80	0.02#
51.00	115.00	0.06#
0.00	0.00	0.00

> 02/10/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (QT Reviewed)

Data File : VW014923.D
Acq On : 07 Feb 2020 16:30
Operator : SY/VA
Sample : L1415-04
Misc : 5.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:42:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
F3S23

Manual Integrations
APPROVED

apatel
2/17/2020 8:51:59 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	866838	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	820838	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	316217	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	236718	16.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.00%
7) Chloroethane-d5	2.89	69	236225	20.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.24%
10) 1,1-Dichloroethene-d2	4.01	63	369780	14.10	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.40%
20) 2-Butanone-d5	7.07	46	172678	42.88	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.76%
24) Chloroform-d	7.65	84	560004	22.75	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	8.30	65	325729m	23.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.68%
29) Benzene-d6	8.27	84	1096464	20.77	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.08%
33) 1,2-Dichloropropane-d6	9.27	67	390105	22.68	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.72%
37) Toluene-d8	10.32	98	925977	19.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.72%
38) trans-1,3-Dichloropropene-	10.58	79	123616	18.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.80%
39) 2-Hexanone-d5	10.92	63	120309	38.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	274630	21.20	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.80%
61) 1,2-Dichlorobenzene-d4	13.85	152	282368	23.03	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.12%

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

202/10/2009