

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (Qedit)




Data File : VW014924.D
Acq On : 07 Feb 2020 16:57
Operator : SY/VA
Sample : L1415-05
Misc : 5.80G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S25

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:30 PM

Quant Time: Feb 08 04:03:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

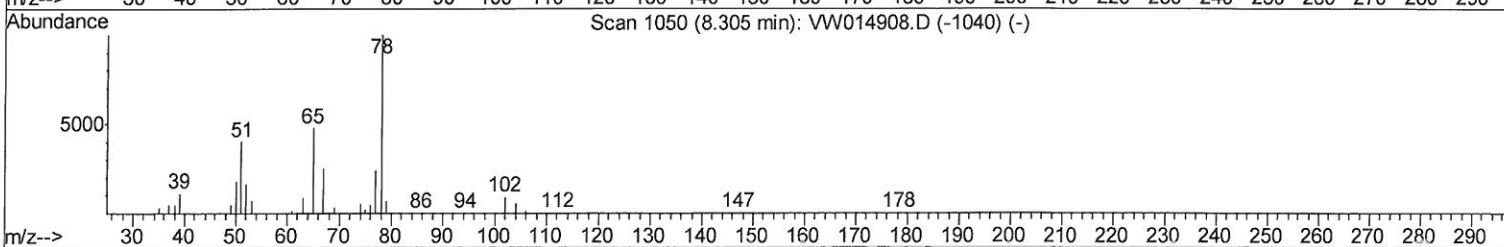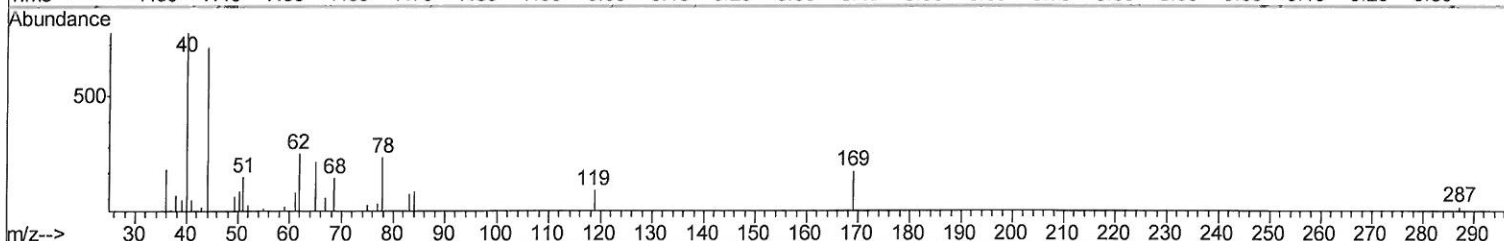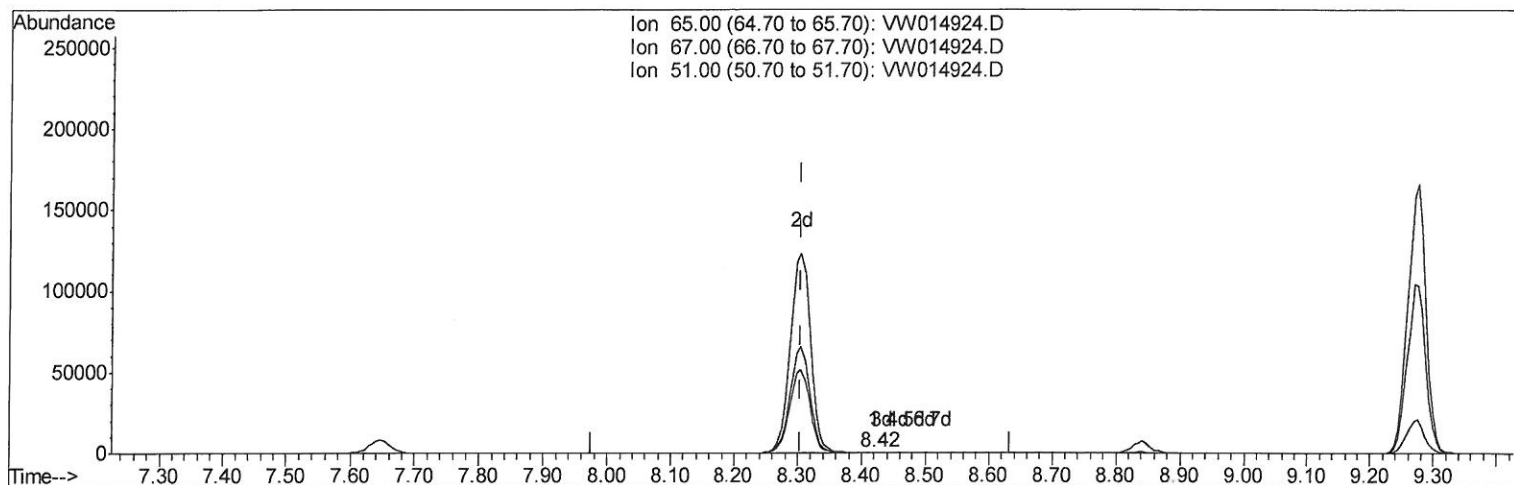

TIC: VW014924.D

(26) 1,2-Dichloroethane-d4 (S)

8.421min (+0.115) 0.01ug/L

response 145

Ion	Exp%	Act%
65.00	100	100
67.00	53.80	48.97
51.00	115.00	96.55
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (Qedit)




Data File : VW014924.D
Acq On : 07 Feb 2020 16:57
Operator : SY/VA
Sample : L1415-05
Misc : 5.80G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
F3S25

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:30 PM

Quant Time: Feb 08 04:03:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

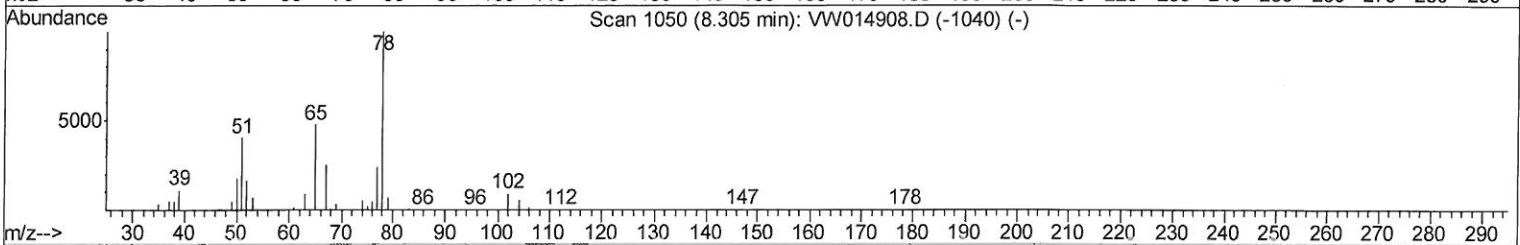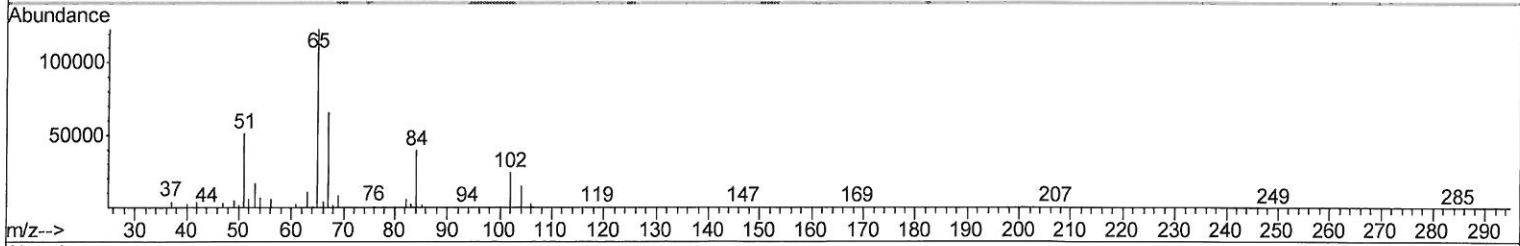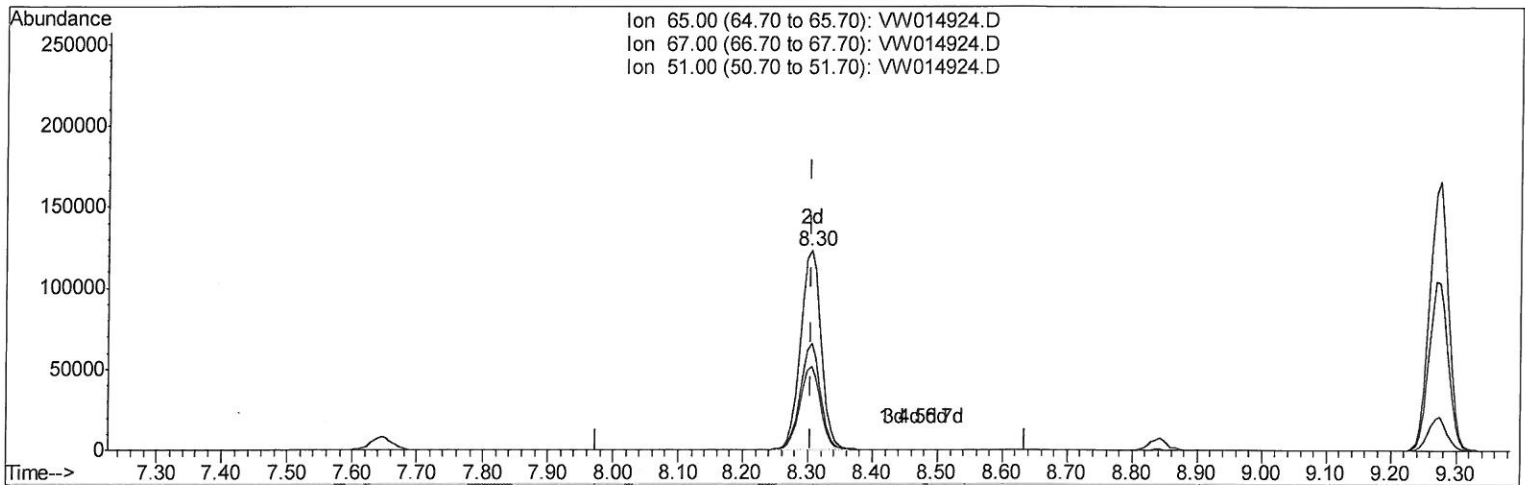

TIC: VW014924.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 27.85ug/L m

response 272187

Ion	Exp%	Act%
65.00	100	100
67.00	53.80	0.03#
51.00	115.00	0.05#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (QT Reviewed)

Data File : VW014924.D
Acq On : 07 Feb 2020 16:57
Operator : SY/VA
Sample : L1415-05
Misc : 5.80G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S25

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:30 PM

Quant Time: Feb 08 05:45:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	622096	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	597584	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	222934	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	202398	19.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.60%
7) Chloroethane-d5	2.89	69	205172	24.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.52%
10) 1,1-Dichloroethene-d2	4.01	63	317576	16.88	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.52%
20) 2-Butanone-d5	7.08	46	138923	48.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.14%
24) Chloroform-d	7.65	84	471999	26.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	106.88%
26) 1,2-Dichloroethane-d4	8.30	65	272187m	27.85	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.40%
29) Benzene-d6	8.27	84	927399	24.13	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.52%
33) 1,2-Dichloropropane-d6	9.27	67	328846	26.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.04%
37) Toluene-d8	10.32	98	772129	22.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.32%
38) trans-1,3-Dichloropropene-	10.58	79	104931	21.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.88%
39) 2-Hexanone-d5	10.92	63	94583	41.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	219271	23.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	236049	27.30	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.20%

Target Compounds				Qvalue
13) Acetone	4.12	43	11939	4.002 ug/L 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (QT Reviewed)

Data File : VW014924.D
Acq On : 07 Feb 2020 16:57
Operator : SY/VA
Sample : L1415-05
Misc : 5.80G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S25

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:30 PM

Quant Time: Feb 08 05:45:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

