

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (Qedit)




Data File : VW014929.D
Acq On : 07 Feb 2020 19:08
Operator : SY/VA
Sample : L1415-10
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S45

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:42 PM

Quant Time: Feb 08 04:04:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

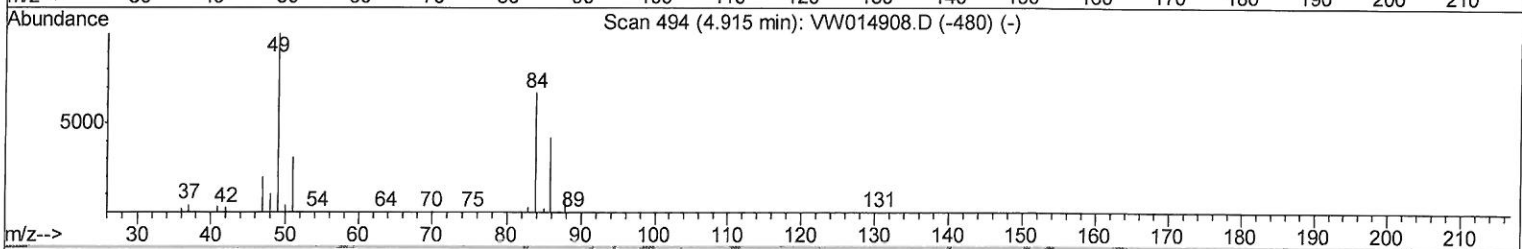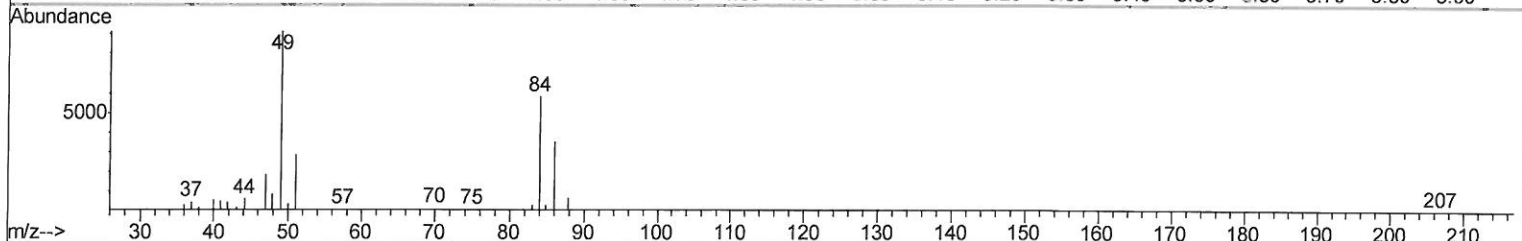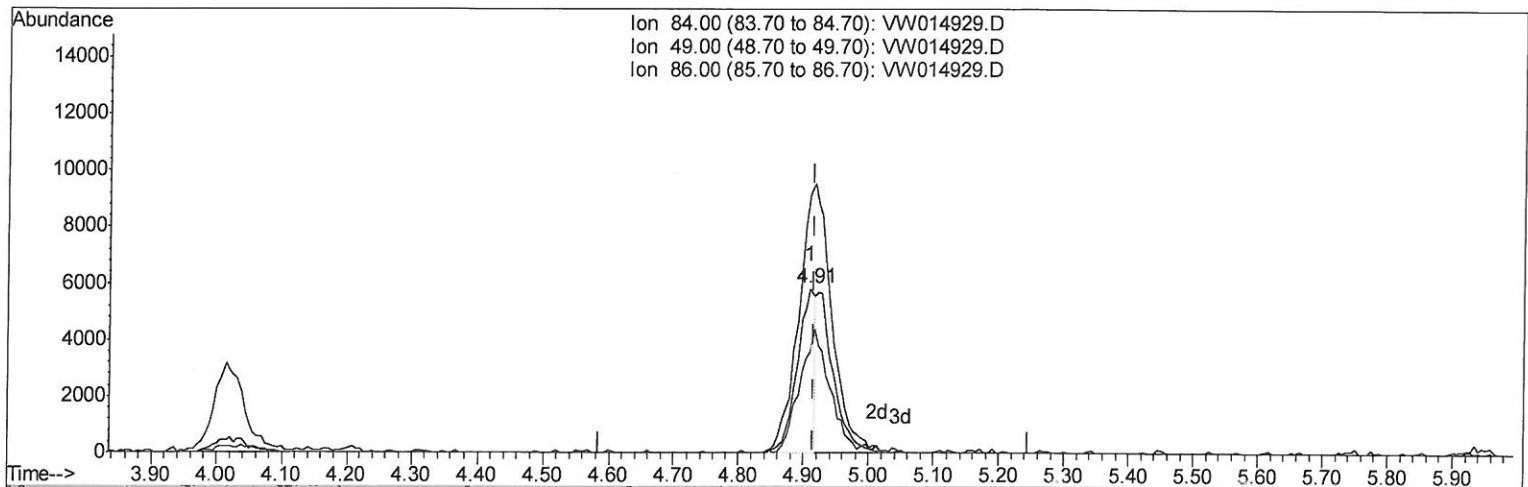

TIC: VW014929.D

(16) Methylene chloride (T)

4.909min (-0.006) 0.89ug/L

response 10850

Ion	Exp%	Act%
84.00	100	100
49.00	136.80	156.92
86.00	63.20	61.19
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020720\
Quantitation Report (Qedit)




Data File : VW014929.D
Acq On : 07 Feb 2020 19:08
Operator : SY/VA
Sample : L1415-10
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S45

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:42 PM

Quant Time: Feb 08 04:04:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

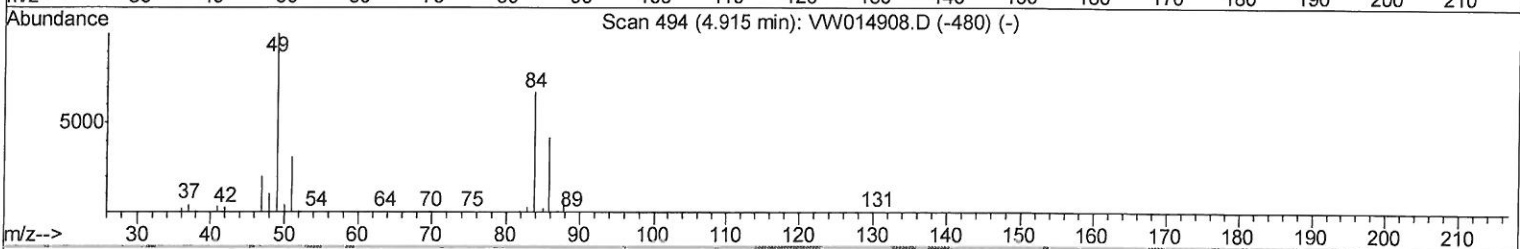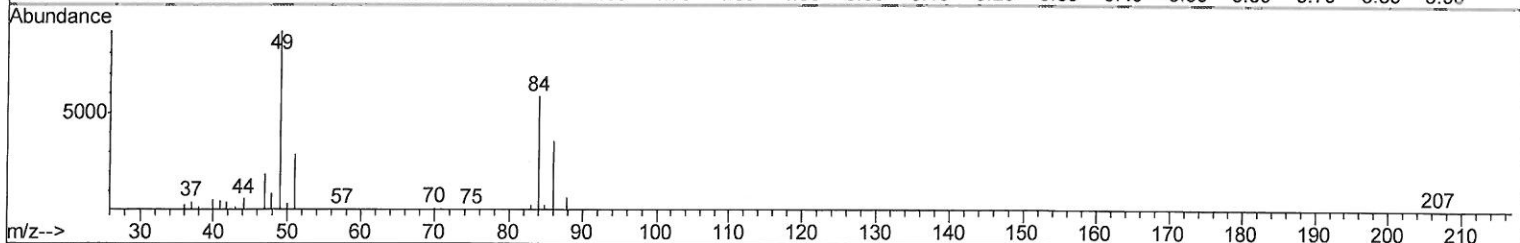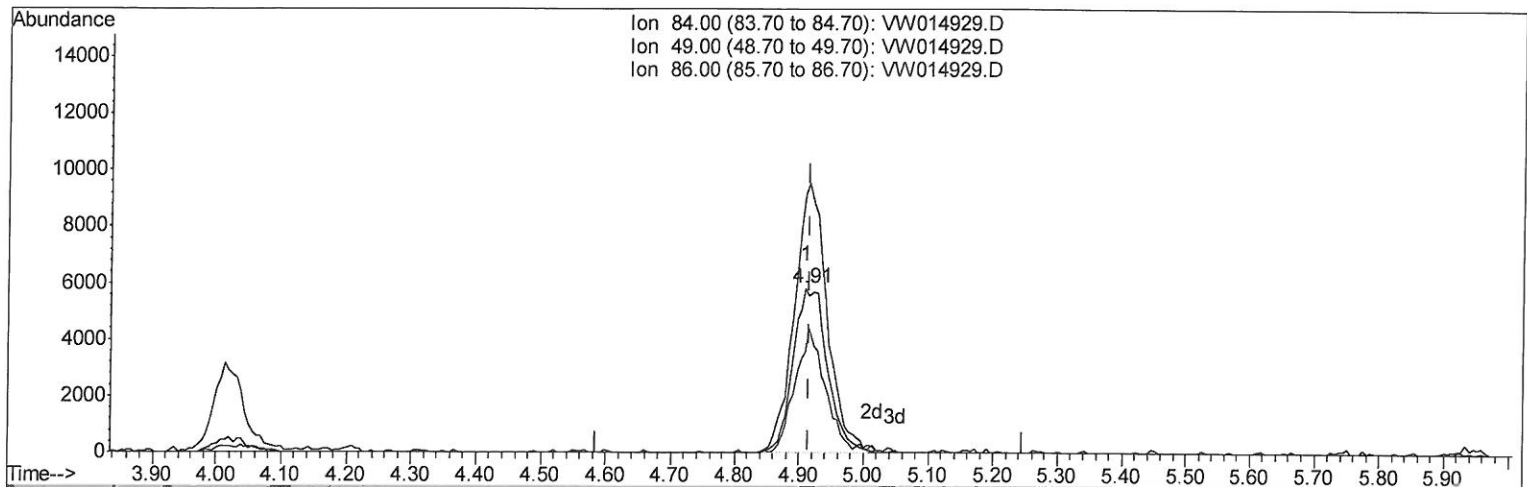

TIC: VW014929.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.74ug/L m

So 2/10/2020

response 21300

Ion	Exp%	Act%
84.00	100	100
49.00	136.80	156.92
86.00	63.20	61.19
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020720\
Quantitation Report (LSC Reviewed)

Data File : VW014929.D
Acq On : 07 Feb 2020 19:08
Operator : SY/VA
Sample : L1415-10
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S45

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:42 PM

Quant Time: Feb 10 11:26:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	672170	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	631953	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	223913	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	199736	17.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.80%
7) Chloroethane-d5	2.89	69	199894	22.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.76%
10) 1,1-Dichloroethene-d2	4.01	63	316790	15.58	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.32%
20) 2-Butanone-d5	7.07	46	127877	40.95	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.90%
24) Chloroform-d	7.65	84	493674	25.87	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.48%
26) 1,2-Dichloroethane-d4	8.30	65	295366	27.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.88%
29) Benzene-d6	8.27	84	944093	23.23	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.92%
33) 1,2-Dichloropropane-d6	9.27	67	345111	26.06	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.24%
37) Toluene-d8	10.32	98	784411	21.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.72%
38) trans-1,3-Dichloropropene-	10.57	79	108512	20.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.00%
39) 2-Hexanone-d5	10.92	63	89410	37.04	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.08%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	234854	23.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.20%
61) 1,2-Dichlorobenzene-d4	13.85	152	217009	24.99	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.96%

Target Compounds

16) Methylene chloride	4.91	84	21300m	1.739	ug/L	Qvalue
------------------------	------	----	--------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020720\
Quantitation Report (LSC Reviewed)

Data File : VW014929.D
Acq On : 07 Feb 2020 19:08
Operator : SY/VA
Sample : L1415-10
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S45

Manual Integrations
APPROVED

MMDadoda
2/10/2020 6:00:42 PM

Quant Time: Feb 10 11:26:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 03:59:50 2020
Response via : Initial Calibration

