
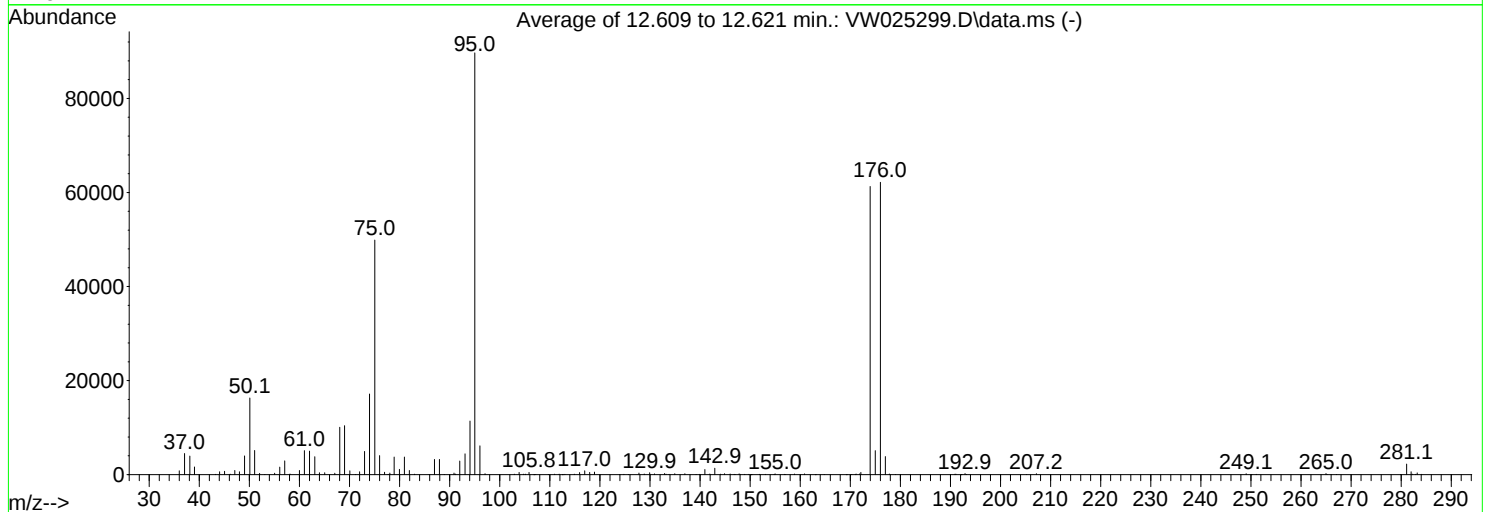


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020723\
Data File : VW025299.D
Acq On : 07 Feb 2023 09:33
Operator : SY/MD
Sample : BFB477
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB477

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Title : SFAM01.0
Last Update : Tue Feb 07 20:11:22 2023

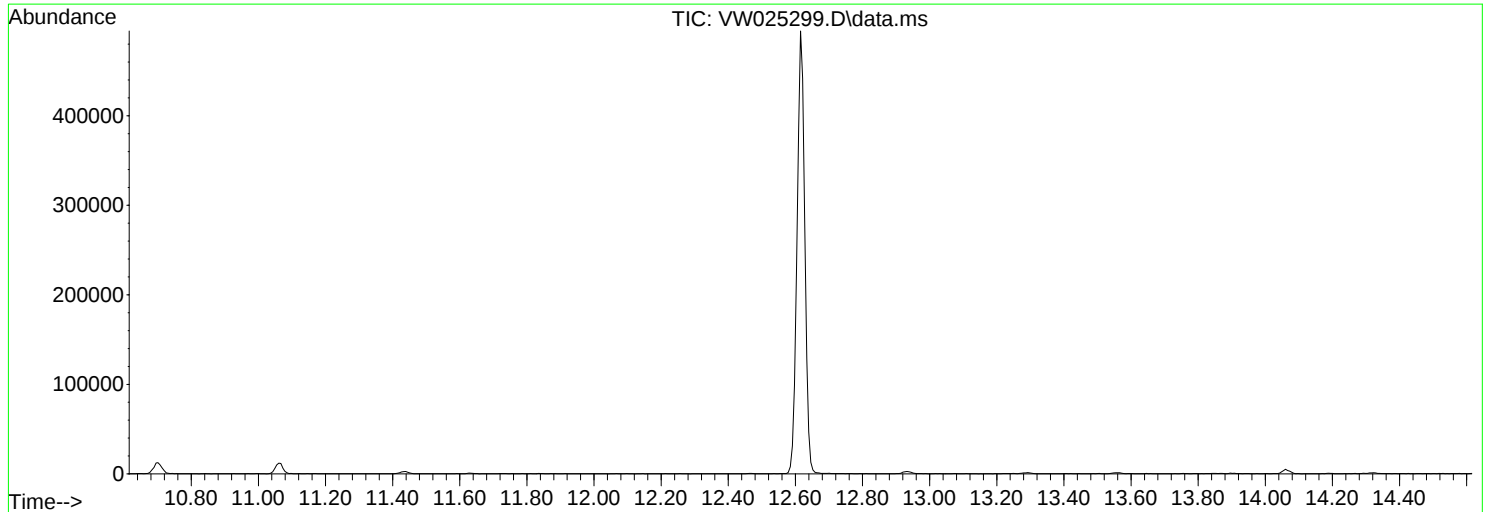

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	16311	PASS
75	95	30	80	55.6	49888	PASS
95	95	100	100	100.0	89699	PASS
96	95	5	9	6.8	6115	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.3	61285	PASS
175	174	5	9	8.3	5112	PASS
176	174	95	105	101.5	62181	PASS
177	176	5	10	6.2	3862	PASS

Scan 1749 (12.567 min): VW025299.D\data.ms
BFB477

m/z	Abundance
39.90	164.0
42.90	61.0
44.10	101.0
57.30	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

m/z	Abundance
36.00	840.0
37.00	4420.0
38.10	3891.0
39.10	1473.0
40.00	164.0
42.80	109.0
43.30	107.0
44.00	552.0
45.00	606.0
46.20	82.0
47.10	823.0
48.00	586.0
49.00	4004.0
50.10	15346.0
51.10	4890.0
52.00	219.0
53.10	71.0
55.00	340.0
56.10	1415.0
57.10	2548.0
58.10	151.0
60.00	705.0
61.00	4304.0
62.00	4521.0
63.10	3758.0
64.00	448.0
65.00	389.0
67.20	355.0
68.00	9235.0
69.00	9437.0
70.10	754.0
71.90	444.0
73.00	4622.0
74.00	16189.0
75.10	45288.0
76.00	3622.0
77.10	429.0
78.00	255.0
78.90	3480.0
80.00	1049.0
81.00	3191.0
82.00	774.0
83.10	89.0
85.90	107.0
87.00	3130.0
87.90	2599.0
91.10	429.0
92.00	2458.0
93.00	3989.0
94.10	10246.0
95.00	79640.0
96.10	4993.0
97.10	262.0
103.00	92.0
103.90	433.0
104.70	95.0
105.20	141.0
105.90	334.0
106.80	50.0
111.00	85.0
111.80	75.0
113.10	50.0
114.80	120.0
115.90	363.0
117.10	600.0
118.00	356.0
118.80	551.0
124.80	84.0
125.70	73.0
127.90	271.0
128.90	80.0
130.00	264.0
130.90	103.0
132.90	337.0
133.20	369.0
133.90	67.0
135.00	148.0
137.00	168.0
139.90	113.0
141.00	806.0
143.00	1224.0
144.20	73.0
144.90	201.0
146.00	142.0
146.80	85.0
147.80	272.0
148.90	77.0
154.80	228.0
156.80	95.0
158.90	133.0
160.80	140.0
163.00	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

164.80	74.0
171.00	143.0
171.90	501.0
174.00	48880.0
175.00	4111.0
176.00	47128.0
177.00	3356.0
177.80	86.0
179.00	60.0
190.90	321.0
192.10	54.0
192.90	363.0
205.20	89.0
207.10	289.0
249.00	244.0
250.00	52.0
251.10	135.0
265.00	377.0
266.00	149.0
267.10	68.0
281.10	3527.0
282.00	1061.0
283.20	647.0
284.10	215.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

m/z	Abundance
35.90	865.0
37.00	4819.0
38.10	4077.0
39.00	1975.0
40.10	155.0
42.90	73.0
44.00	864.0
45.00	888.0
46.10	142.0
47.10	990.0
48.00	686.0
49.00	4207.0
50.10	17752.0
51.10	5789.0
52.10	276.0
55.10	346.0
56.10	1792.0
57.00	3560.0
58.10	131.0
60.00	1082.0
61.00	6212.0
62.00	5402.0
63.00	3829.0
64.00	446.0
65.10	559.0
67.00	323.0
68.10	11021.0
69.00	11759.0
70.00	907.0
72.00	775.0
73.00	5638.0
74.00	18424.0
75.00	54944.0
76.00	4399.0
76.90	602.0
78.00	427.0
78.90	4173.0
79.90	1321.0
80.90	4400.0
81.90	952.0
83.10	88.0
85.90	59.0
86.90	3220.0
88.00	4174.0
88.90	95.0
90.80	578.0
92.00	3577.0
93.10	4900.0
94.10	12761.0
95.00	102080.0
96.10	6920.0
97.10	195.0
102.80	129.0
103.80	475.0
105.00	190.0
105.80	549.0
109.70	68.0
110.90	87.0
111.80	62.0
112.50	58.0
113.00	86.0
114.90	137.0
116.00	453.0
116.90	858.0
117.90	581.0
118.90	709.0
123.90	88.0
124.80	112.0
127.70	353.0
128.90	151.0
129.90	430.0
131.00	161.0
132.90	293.0
133.70	94.0
135.00	288.0
137.00	234.0
139.90	78.0
140.90	1422.0
141.90	184.0
142.90	1463.0
144.10	60.0
144.90	263.0
145.90	153.0
146.80	87.0
147.80	236.0
148.80	70.0
149.70	89.0
150.20	57.0
151.90	93.0
153.00	76.0
155.00	321.0
157.10	117.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

158.80	173.0
160.90	236.0
171.20	231.0
172.10	821.0
174.00	70576.0
175.00	5565.0
176.00	70560.0
177.00	4382.0
177.80	195.0
179.00	64.0
191.10	183.0
192.90	393.0
207.10	137.0
249.10	228.0
265.00	304.0
279.90	58.0
281.10	2302.0
282.00	740.0
283.20	500.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

m/z	Abundance
36.10	784.0
37.10	4256.0
38.10	3929.0
39.10	1439.0
40.00	127.0
43.20	115.0
44.10	731.0
45.10	689.0
46.10	107.0
47.10	813.0
48.00	594.0
49.10	3697.0
50.10	15835.0
51.00	4777.0
52.10	316.0
55.00	283.0
56.00	1645.0
57.00	2710.0
58.00	89.0
60.00	910.0
61.00	4798.0
62.00	5088.0
63.10	3857.0
64.00	369.0
65.10	309.0
67.00	260.0
68.00	9912.0
69.00	10059.0
70.00	831.0
71.20	100.0
72.10	605.0
73.00	4576.0
74.00	16824.0
75.00	49432.0
76.00	4177.0
77.00	546.0
77.70	241.0
78.10	326.0
78.90	3552.0
80.00	1053.0
81.00	3660.0
81.90	894.0
82.90	122.0
87.00	3312.0
87.90	2959.0
90.90	406.0
92.00	2657.0
93.00	4441.0
94.00	11248.0
95.00	87376.0
96.00	6432.0
96.90	159.0
102.90	108.0
103.90	522.0
104.80	196.0
105.90	559.0
107.20	95.0
109.70	77.0
111.00	148.0
111.90	135.0
112.90	102.0
115.00	112.0
116.00	488.0
116.90	988.0
117.90	484.0
119.00	406.0
124.00	59.0
127.80	417.0
128.80	161.0
129.90	538.0
130.80	257.0
133.00	102.0
133.80	79.0
134.90	182.0
136.90	185.0
139.20	82.0
139.90	64.0
141.00	1052.0
142.00	246.0
142.90	1399.0
144.10	178.0
144.90	160.0
146.10	133.0
147.00	62.0
148.00	228.0
149.00	75.0
149.80	107.0
151.80	108.0
153.10	163.0
155.00	251.0
156.90	111.0
158.80	126.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477

160.90	144.0
169.20	54.0
170.30	85.0
171.10	145.0
172.10	653.0
173.90	64400.0
175.00	5661.0
176.00	68856.0
177.00	3848.0
177.80	130.0
191.10	85.0
193.20	152.0
207.20	156.0
249.00	110.0
250.90	66.0
265.20	121.0
279.90	65.0
281.10	952.0
282.20	314.0
282.90	201.0

Instrument :
MSVOA_W
ClientSampleId :
BFB477