

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020923\
 Data File : VW025320.D
 Acq On : 09 Feb 2023 10:07
 Operator : SY/MD
 Sample : VW0209SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK462

Quant Time: Feb 10 00:30:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 07 20:11:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	382594	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	339347	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	157830	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.368	65	82402	22.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.040%
7) Chloroethane-d5	2.898	69	62908	19.136	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.560%
11) 1,1-Dichloroethene-d2	4.026	63	165795	16.150	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.600%
21) 2-Butanone-d5	7.074	46	49198	51.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.380%
24) Chloroform-d	7.647	84	245402	24.472	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.880%
26) 1,2-Dichloroethane-d4	8.306	65	127319	26.065	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.280%
32) Benzene-d6	8.275	84	485810	23.620	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.480%
36) 1,2-Dichloropropane-d6	9.275	67	140281	23.311	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.240%
41) Toluene-d8	10.324	98	447400	24.335	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.360%
43) trans-1,3-Dichloroprop...	10.574	79	56482	25.118	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.480%
47) 2-Hexanone-d5	10.921	63	38206	56.625	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.260%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	101404	24.779	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.120%
66) 1,2-Dichlorobenzene-d4	13.847	152	141360	25.815	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.280%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	12269	1.865	ug/L	# 5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020923\
Data File : VW025320.D
Acq On : 09 Feb 2023 10:07
Operator : SY/MD
Sample : VW0209SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK462


Quant Time: Feb 10 00:30:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 07 20:11:22 2023
Response via : Initial Calibration

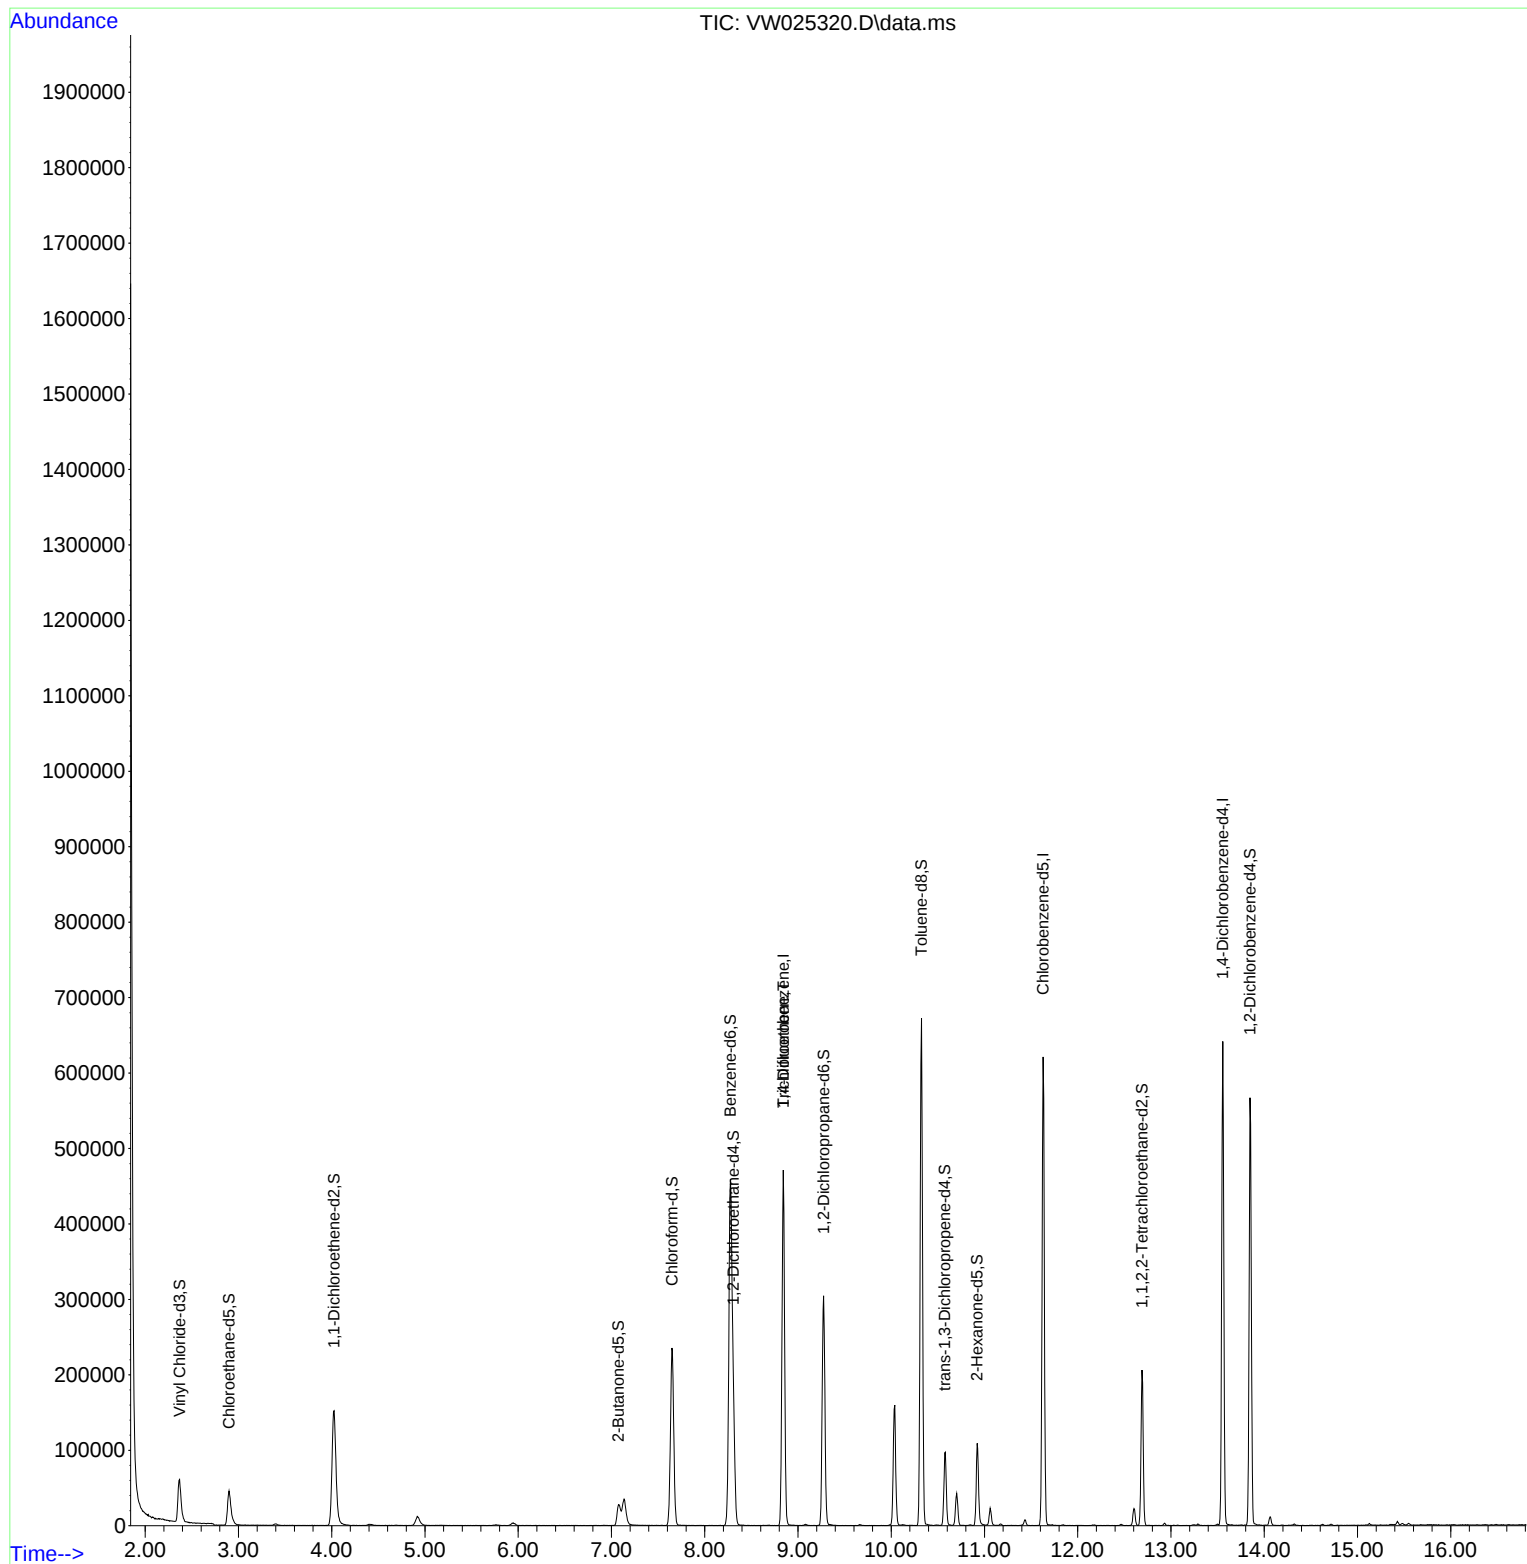

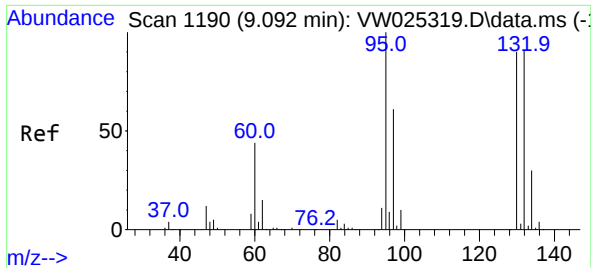

#34
 Trichloroethene
 Concen: 1.865 ug/L
 RT: 8.842 min Scan# 11
 Delta R.T. -0.249 min
 Lab File: VW025320.D
 Acq: 09 Feb 2023 10:07

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK462

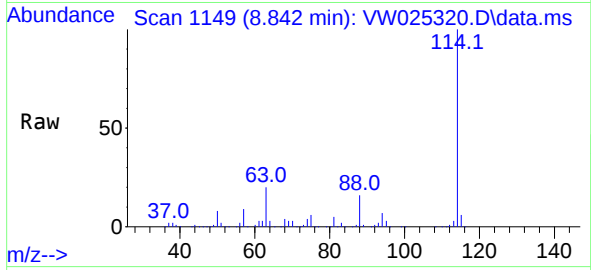

Tgt Ion: 95 Resp: 12269

Ion	Ratio	Lower	Upper
95	100		
97	0.0	45.4	84.2#
132	0.0	67.1	124.5#
130	0.0	69.2	128.6#

