


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020923\
Data File : VW025318.D
Acq On : 09 Feb 2023 07:41
Operator : SY/MD
Sample : BFB479
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB479

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Title : SFAM01.0
Last Update : Tue Feb 07 20:11:22 2023

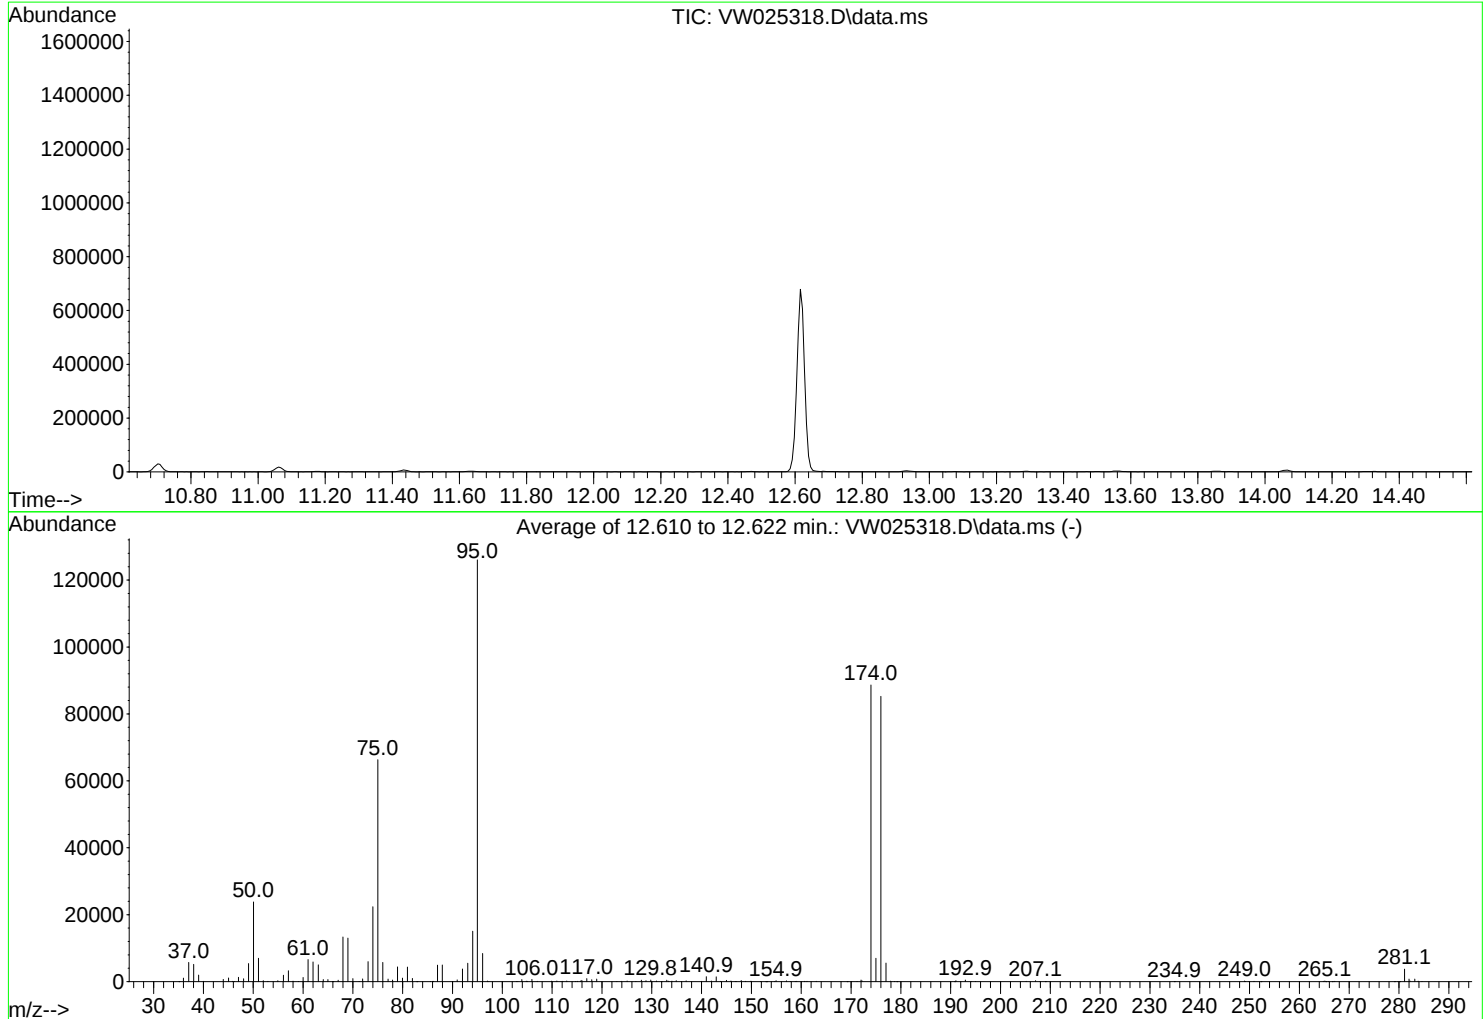

AutoFind: Scans 1767, 1768, 1769; Background Corrected with Scan 1760

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	23805	PASS
75	95	30	80	52.6	66312	PASS
95	95	100	100	100.0	126045	PASS
96	95	5	9	6.7	8409	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.3	88643	PASS
175	174	5	9	7.9	6965	PASS
176	174	95	105	96.2	85245	PASS
177	176	5	10	6.5	5541	PASS

m/z	Abundance
40.00	156.0
43.10	87.0
44.00	152.0
55.10	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479

m/z	Abundance
36.00	1080.0
37.10	4881.0
38.00	4532.0
39.10	1881.0
40.10	263.0
43.20	73.0
44.10	769.0
45.10	1047.0
46.20	140.0
47.00	1309.0
48.00	768.0
49.10	4929.0
50.10	21200.0
51.00	6777.0
52.00	281.0
52.90	79.0
55.20	221.0
56.10	1611.0
57.10	2963.0
58.00	138.0
59.10	132.0
60.00	1123.0
61.00	6412.0
62.00	5519.0
63.10	4576.0
64.10	637.0
65.00	645.0
66.30	56.0
67.00	324.0
68.00	11957.0
69.00	11576.0
70.00	901.0
72.00	842.0
73.10	5054.0
74.00	19808.0
75.00	57816.0
76.00	5557.0
77.00	789.0
78.00	455.0
79.00	4032.0
80.00	1073.0
80.90	3869.0
82.00	813.0
83.10	64.0
86.00	247.0
87.00	4712.0
88.00	4908.0
90.90	357.0
92.00	3084.0
93.00	4756.0
94.10	12345.0
95.00	112872.0
96.00	7736.0
97.10	243.0
103.10	127.0
104.00	632.0
104.80	296.0
106.00	644.0
107.00	133.0
109.90	120.0
111.00	220.0
111.80	119.0
112.90	246.0
114.70	61.0
115.10	92.0
115.90	443.0
116.90	715.0
117.90	558.0
119.00	779.0
123.80	116.0
125.00	227.0
126.80	120.0
127.90	309.0
128.80	220.0
129.80	472.0
131.00	196.0
131.90	52.0
133.00	613.0
133.40	464.0
134.10	210.0
134.90	303.0
136.00	60.0
136.90	228.0
140.90	1003.0
142.10	178.0
142.90	984.0
143.90	66.0
145.10	488.0
145.90	129.0
146.70	129.0
147.00	148.0
147.90	344.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479

148.90	62.0
149.80	103.0
152.90	78.0
154.70	209.0
155.00	218.0
157.10	274.0
159.20	154.0
160.80	157.0
161.20	110.0
163.10	108.0
172.00	579.0
174.00	69840.0
175.00	6022.0
176.00	62192.0
177.00	4344.0
178.00	198.0
178.80	109.0
191.00	418.0
193.00	789.0
194.10	92.0
195.00	124.0
205.10	176.0
207.00	448.0
207.90	59.0
209.00	87.0
234.90	81.0
249.00	348.0
250.90	161.0
252.30	60.0
265.10	620.0
265.90	123.0
266.60	51.0
267.10	165.0
279.10	84.0
279.80	125.0
281.10	5628.0
282.00	1453.0
283.10	1364.0
283.90	254.0
284.60	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479

m/z	Abundance
36.00	1084.0
37.00	6651.0
38.10	5956.0
39.10	2171.0
40.00	285.0
43.30	74.0
44.00	910.0
45.10	1343.0
45.90	174.0
47.10	1543.0
48.10	779.0
49.00	5855.0
50.00	27552.0
51.00	7575.0
52.00	413.0
53.00	129.0
54.90	382.0
56.00	2347.0
57.00	3597.0
58.00	208.0
60.00	1494.0
61.00	7079.0
62.00	6200.0
63.00	5629.0
64.00	668.0
65.10	722.0
65.90	84.0
67.10	439.0
68.00	15443.0
69.00	14740.0
70.00	1090.0
71.20	100.0
71.90	927.0
73.00	6479.0
74.00	25224.0
75.00	74944.0
76.00	6574.0
77.00	842.0
77.90	480.0
78.90	4907.0
79.90	1114.0
80.90	4891.0
81.90	1037.0
82.80	84.0
85.60	202.0
87.00	5056.0
87.90	4875.0
91.00	557.0
92.00	4231.0
93.10	6272.0
94.10	17240.0
95.00	140032.0
96.10	9446.0
97.00	245.0
102.80	65.0
103.80	588.0
105.00	312.0
106.00	791.0
107.00	123.0
109.80	213.0
111.00	133.0
112.10	134.0
112.90	161.0
115.00	221.0
116.00	738.0
117.00	1176.0
118.00	663.0
118.90	706.0
123.00	55.0
123.90	168.0
125.10	189.0
126.80	83.0
127.90	479.0
128.80	376.0
129.80	501.0
130.90	236.0
133.00	397.0
134.00	142.0
134.90	244.0
135.90	117.0
136.90	211.0
139.90	162.0
141.00	1732.0
141.90	263.0
142.90	1820.0
143.70	113.0
144.90	327.0
145.90	253.0
146.80	102.0
147.90	383.0
148.80	139.0
149.90	183.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479

151.90	56.0
153.10	77.0
154.90	286.0
156.90	192.0
157.10	190.0
157.90	53.0
159.00	141.0
161.10	219.0
163.00	90.0
170.10	110.0
172.20	673.0
174.00	102056.0
175.00	7054.0
176.00	99960.0
177.00	6405.0
177.90	285.0
178.70	100.0
179.20	82.0
191.10	405.0
192.00	142.0
192.90	387.0
194.10	87.0
195.00	61.0
205.20	65.0
207.10	280.0
208.00	76.0
249.00	311.0
250.90	86.0
264.80	289.0
265.80	111.0
267.10	75.0
281.00	3602.0
282.00	843.0
283.20	691.0
283.80	255.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479

m/z	Abundance
35.10	57.0
36.00	983.0
37.10	5629.0
38.10	5014.0
39.00	1917.0
40.00	195.0
43.90	760.0
45.00	982.0
45.80	71.0
47.00	1002.0
48.00	990.0
49.10	5387.0
50.00	22664.0
51.10	6617.0
52.00	246.0
52.90	161.0
55.00	445.0
56.00	1780.0
57.10	3179.0
58.00	102.0
60.00	1077.0
61.00	6306.0
62.00	5872.0
63.00	4867.0
64.00	537.0
64.90	500.0
66.10	95.0
67.10	475.0
68.00	12599.0
69.00	12735.0
70.00	781.0
71.30	86.0
72.00	686.0
73.00	6394.0
74.00	22064.0
75.00	66176.0
76.00	5121.0
77.10	699.0
78.00	508.0
78.90	4215.0
79.90	1035.0
81.00	4251.0
82.00	985.0
83.00	168.0
86.20	264.0
87.00	5034.0
88.00	5076.0
90.90	659.0
92.00	3988.0
93.00	5504.0
94.00	15555.0
95.00	125232.0
96.10	8044.0
96.90	177.0
97.30	151.0
102.90	60.0
103.90	626.0
104.80	181.0
105.80	525.0
107.10	64.0
109.70	83.0
110.00	76.0
110.90	188.0
112.20	142.0
113.00	170.0
114.70	166.0
115.70	555.0
117.00	896.0
118.00	536.0
118.90	795.0
123.00	98.0
123.90	53.0
125.00	124.0
127.90	476.0
128.90	249.0
129.80	463.0
131.00	151.0
133.00	213.0
133.90	60.0
134.90	280.0
136.90	325.0
140.00	83.0
141.00	1681.0
141.80	140.0
143.00	1472.0
143.90	108.0
145.00	356.0
145.90	150.0
146.90	63.0
148.00	350.0
148.90	79.0
150.00	159.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479

151.80	83.0
154.90	389.0
157.10	121.0
157.70	87.0
158.80	147.0
160.60	162.0
162.90	53.0
169.20	50.0
171.20	202.0
172.00	821.0
174.00	94032.0
175.00	7818.0
176.00	93584.0
177.00	5874.0
190.80	71.0
191.20	71.0
193.00	310.0
207.00	109.0
249.20	120.0
249.90	168.0
251.00	68.0
264.80	59.0
265.30	91.0
280.10	69.0
281.20	1968.0
282.20	645.0
283.20	311.0

Instrument :
MSVOA_W
ClientSampleId :
BFB479