

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021020\
 Data File : VW014949.D
 Acq On : 10 Feb 2020 18:03
 Operator : SY/VA
 Sample : L1416-06
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F3S34

Manual Integrations
 APPROVED

MMDadoda
 2/11/2020 6:10:35 PM

Quant Time: Feb 11 00:34:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 11 00:31:29 2020
 Response via : Initial Calibration

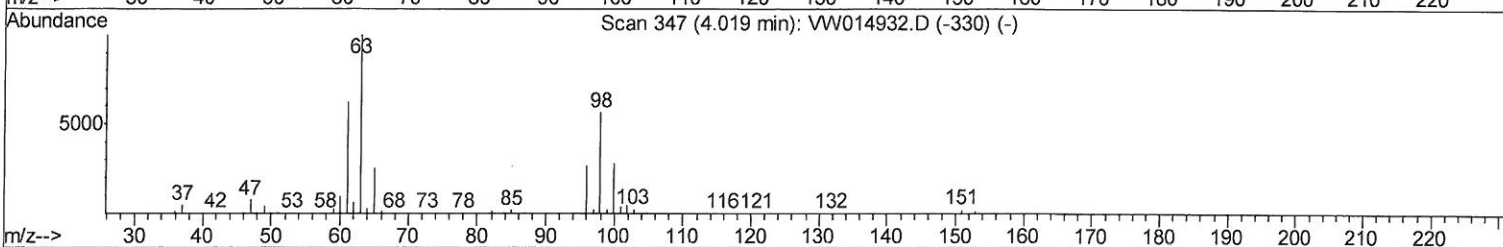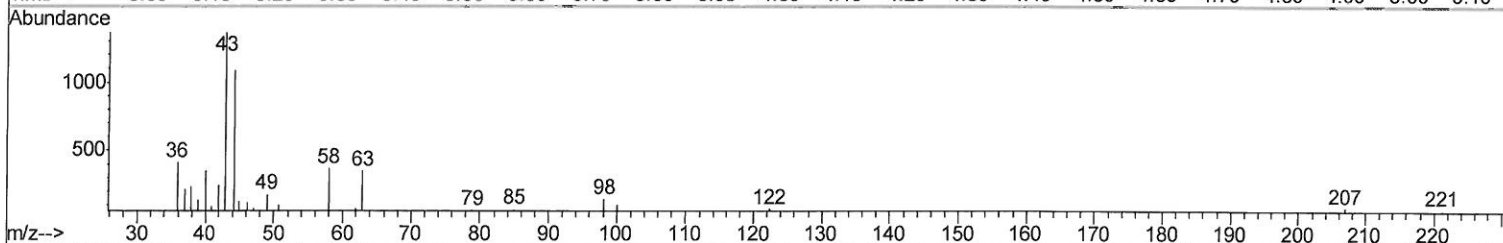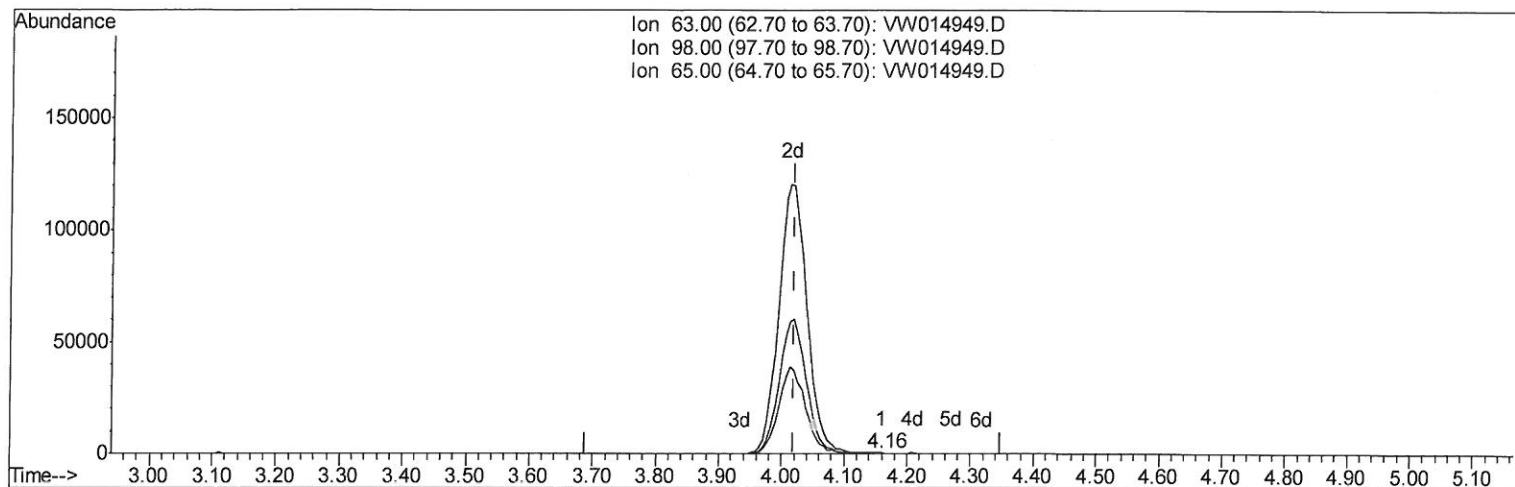

TIC: VW014949.D

(10) 1,1-Dichloroethene-d2 (S)

4.160min (+0.141) 0.01ug/L

response 318

Ion	Exp%	Act%
63.00	100	100
98.00	68.60	70.44
65.00	23.10	29.56
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021020\
 Data File : VW014949.D
 Acq On : 10 Feb 2020 18:03
 Operator : SY/VA
 Sample : L1416-06
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F3S34

Manual Integrations
 APPROVED

MMDadoda
 2/11/2020 6:10:35 PM

Quant Time: Feb 11 00:34:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 11 00:31:29 2020
 Response via : Initial Calibration

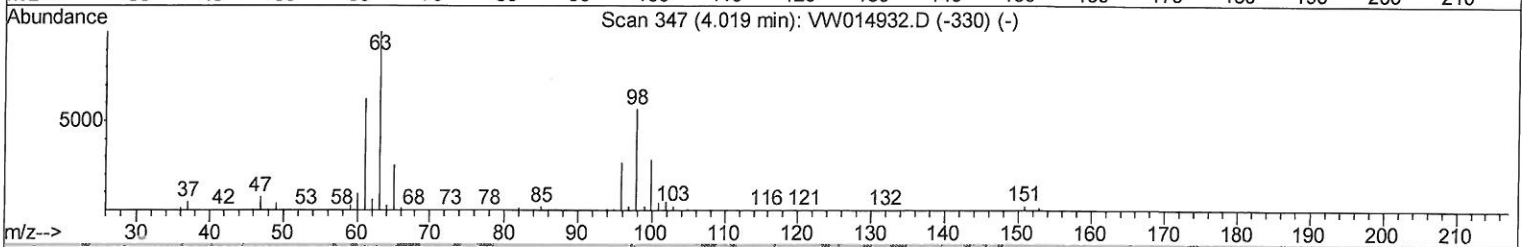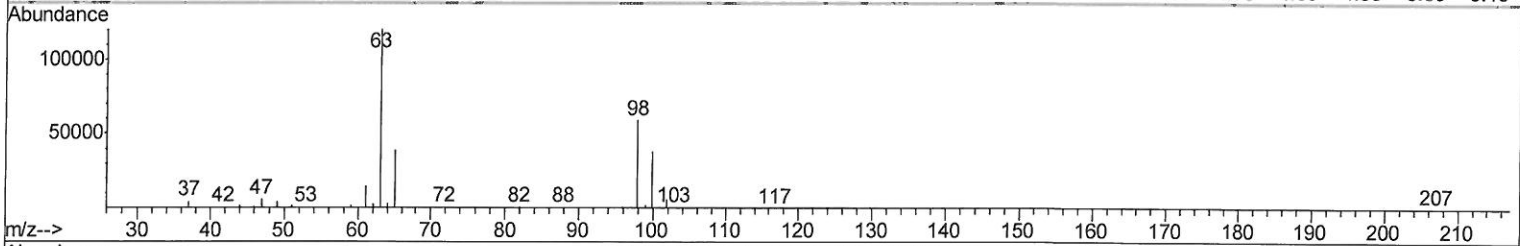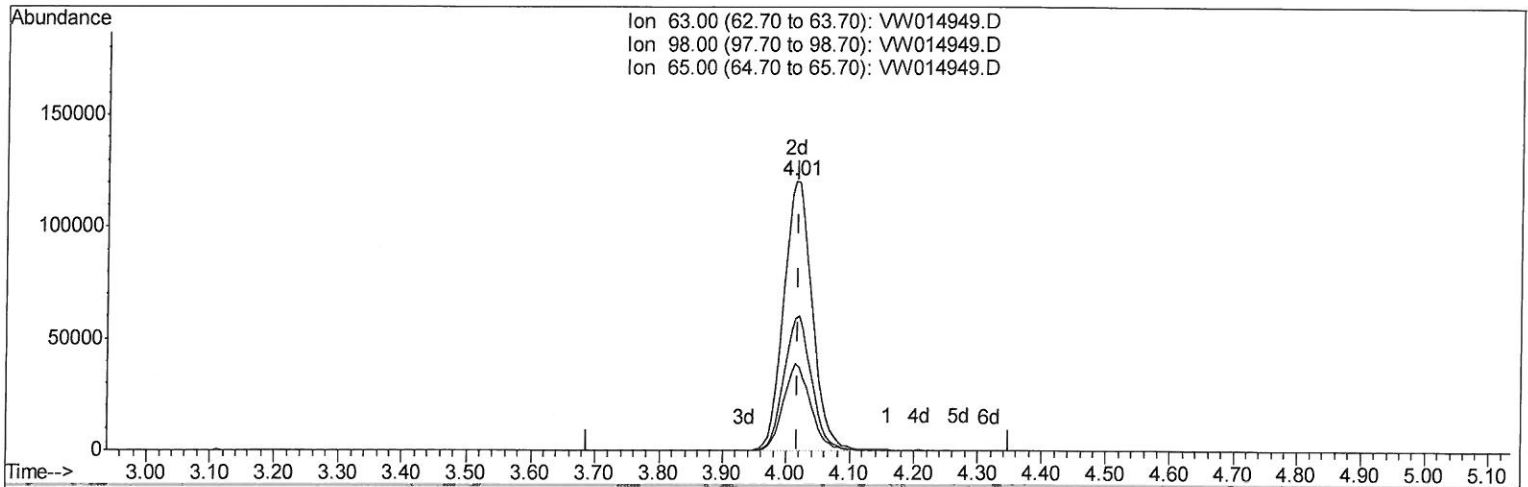

TIC: VW014949.D

(10) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 16.37ug/L m

02/11/2020

response 374855

Ion	Exp%	Act%
63.00	100	100
98.00	68.60	0.06#
65.00	23.10	0.03#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021020\
 Data File : VW014949.D
 Acq On : 10 Feb 2020 18:03
 Operator : SY/VA
 Sample : L1416-06
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F3S34

Manual Integrations
 APPROVED

MMDadoda
 2/11/2020 6:10:35 PM

Quant Time: Feb 11 02:30:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 11 00:31:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	757017	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	685351	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	225950	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	228584	18.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.96%
7) Chloroethane-d5	2.89	69	235070	23.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.72%
10) 1,1-Dichloroethene-d2	4.01	63	374855m	16.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.48%
20) 2-Butanone-d5	7.07	46	181389	51.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.14%
24) Chloroform-d	7.65	84	587465	27.33	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	109.32%
26) 1,2-Dichloroethane-d4	8.31	65	350279	29.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	117.80%
29) Benzene-d6	8.27	84	1102837	25.02	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.08%
33) 1,2-Dichloropropane-d6	9.27	67	407845	28.40	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.60%
37) Toluene-d8	10.32	98	901597	23.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.96%
38) trans-1,3-Dichloropropene-	10.57	79	126438	22.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.16%
39) 2-Hexanone-d5	10.92	63	121264	46.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.64%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	281751	26.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.20%
61) 1,2-Dichlorobenzene-d4	13.85	152	231913	26.47	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.88%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.12	43	13474	3.711	ug/L	68
16) Methylene chloride	4.91	84	35525	2.576	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021020\
Data File : VW014949.D
Acq On : 10 Feb 2020 18:03
Operator : SY/VA
Sample : L1416-06
Misc : 5.36G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F3S34

Manual Integrations
APPROVED

MMDadoda
2/11/2020 6:10:35 PM

Quant Time: Feb 11 02:30:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 11 00:31:29 2020
Response via : Initial Calibration

