

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021020\
 Data File : VW014946.D
 Acq On : 10 Feb 2020 16:45
 Operator : SY/VA
 Sample : L1416-03
 Misc : 4.59G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F3S31

Manual Integrations
 APPROVED

MMDadoda
 2/11/2020 6:10:29 PM

Quant Time: Feb 11 02:09:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 11 00:31:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	853016	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	782693	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	292566	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	249613	17.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.72%
7) Chloroethane-d5	2.89	69	247653	21.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.60%
10) 1,1-Dichloroethene-d2	4.01	63	408428	15.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.32%
20) 2-Butanone-d5	7.07	46	173094	43.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.36%
24) Chloroform-d	7.65	84	599205m	24.74	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.96%
26) 1,2-Dichloroethane-d4	8.31	65	341141	25.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.80%
29) Benzene-d6	8.27	84	1160460	23.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.24%
33) 1,2-Dichloropropane-d6	9.27	67	418044	25.49	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.96%
37) Toluene-d8	10.32	98	974727	22.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.00%
38) trans-1,3-Dichloropropene-	10.58	79	128070	19.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.08%
39) 2-Hexanone-d5	10.92	63	116922	39.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.22%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	265084	21.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.84%
61) 1,2-Dichlorobenzene-d4	13.85	152	276236	24.35	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.40%

Target Compounds					Ovalue
13) Acetone	4.13	43	20859	5.099 ug/L	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW021020\
Data File : VW014946.D
Acq On : 10 Feb 2020 16:45
Operator : SY/VA
Sample : L1416-03
Misc : 4.59G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F3S31

Manual Integrations
APPROVED

MMDadoda
2/11/2020 6:10:29 PM

Quant Time: Feb 11 02:09:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 11 00:31:29 2020
Response via : Initial Calibration

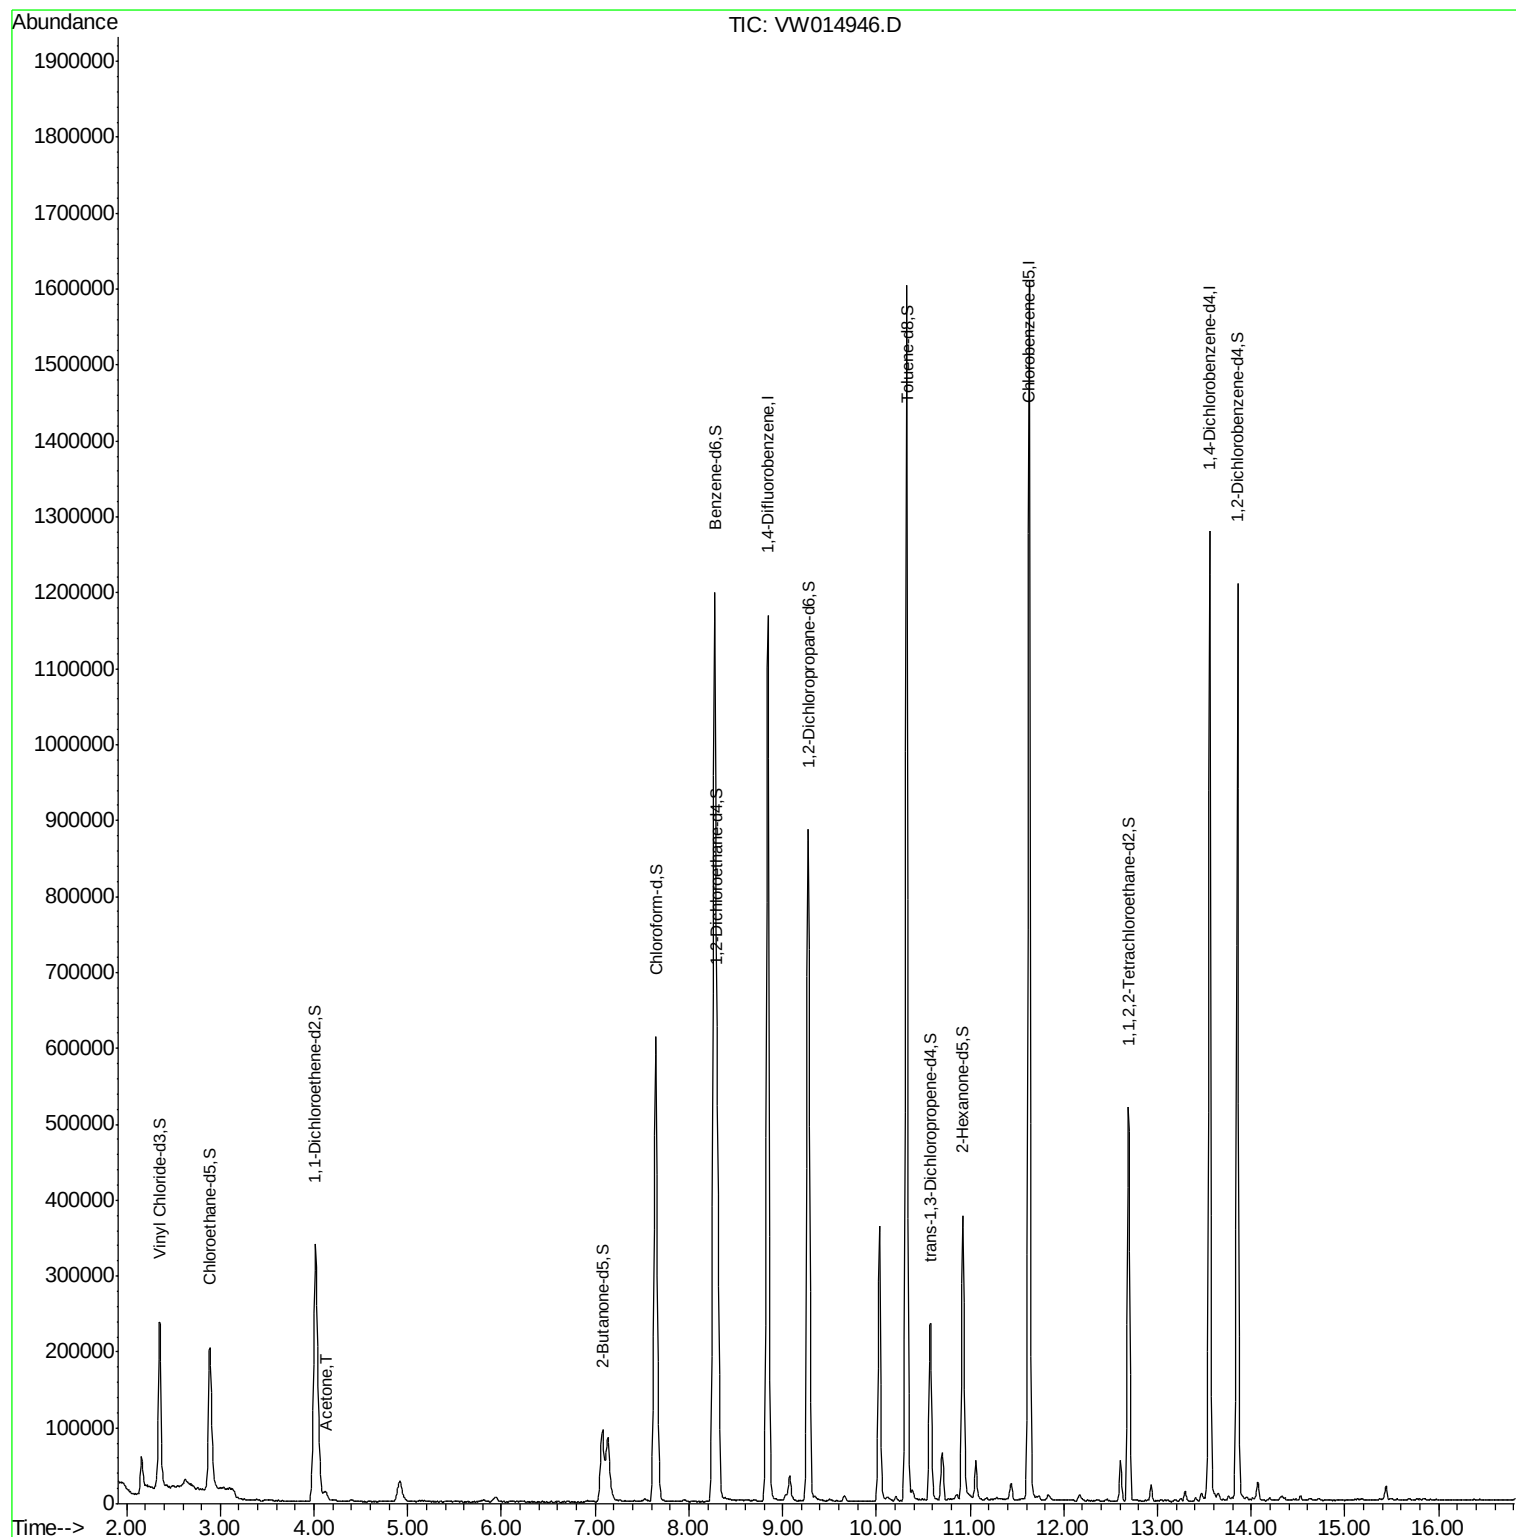

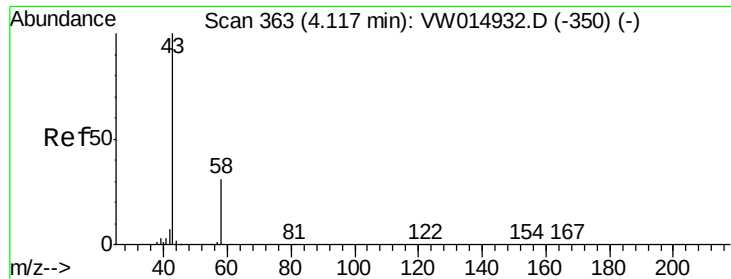

#13
 Acetone
 Concen: 5.099 ug/L
 RT: 4.13 min Scan# 365
 Delta R.T. 0.01 min
 Lab File: VW014946.D
 Acq: 10 Feb 2020 16:45

Instrument :
 MSVOA_W
 ClientSampleId :
 F3S31

Tot Ion	Ratio	Lower	Upper
43	100		
58	16.7	0.0	60.4

Manual Integrations
 APPROVED

MMDadoda
 2/11/2020 6:10:29 PM

