
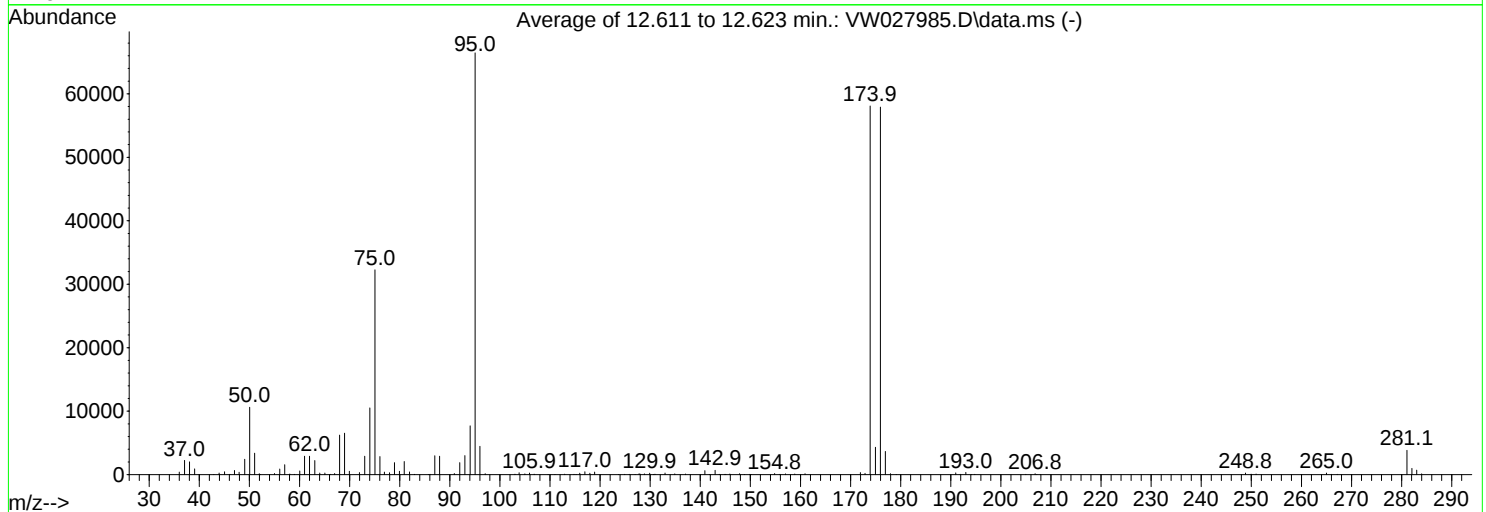


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021224\
Data File : VW027985.D
Acq On : 12 Feb 2024 08:20
Operator : SY/MD
Sample : BFB435
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB435

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Tue Feb 13 00:01:14 2024

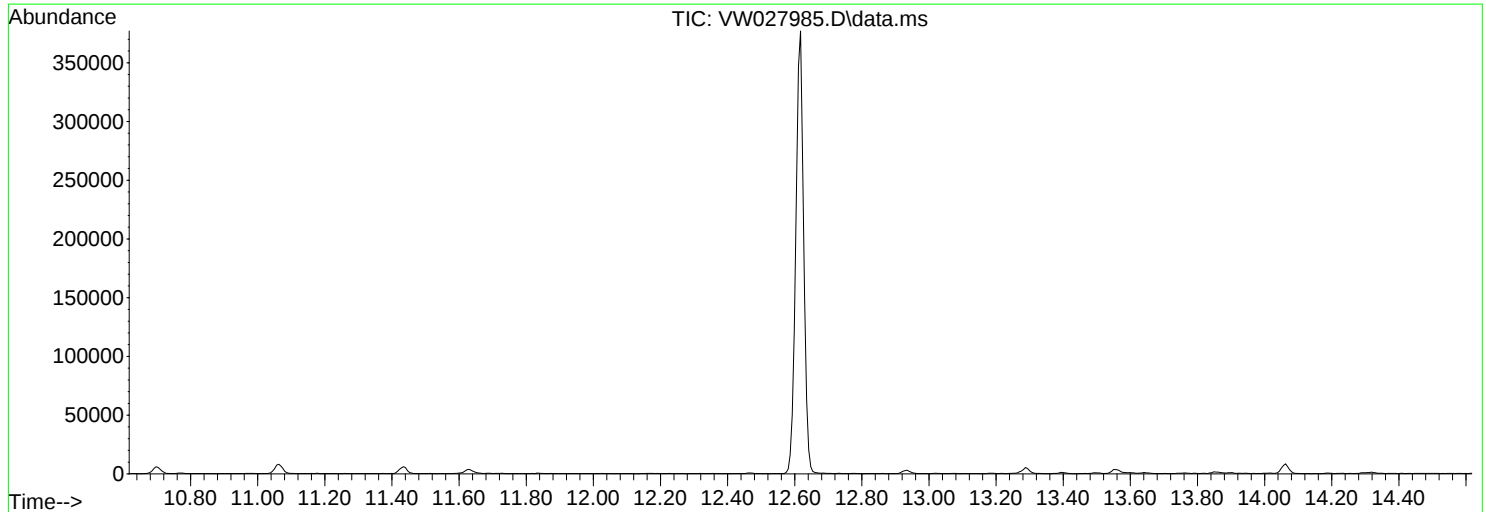

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	10615	PASS
75	95	30	80	48.6	32277	PASS
95	95	100	100	100.0	66461	PASS
96	95	5	9	6.7	4468	PASS
173	174	0.00	2	0.4	204	PASS
174	95	50	120	87.4	58099	PASS
175	174	5	9	7.4	4305	PASS
176	174	95	101	99.7	57923	PASS
177	176	5	9	6.3	3665	PASS

m/z	Abundance
40.00	139.0
43.90	132.0
281.20	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

m/z	Abundance
36.00	444.0
37.10	2335.0
38.00	2417.0
39.10	1043.0
40.00	144.0
42.90	96.0
44.00	434.0
45.00	583.0
46.10	92.0
47.00	747.0
47.90	379.0
49.00	2629.0
50.10	11173.0
51.10	3693.0
52.00	108.0
52.20	110.0
55.00	157.0
56.00	1041.0
57.00	1837.0
58.10	138.0
59.00	70.0
60.00	689.0
61.00	3224.0
62.00	2933.0
63.10	2509.0
64.00	297.0
65.00	267.0
66.10	80.0
67.00	182.0
68.00	6783.0
69.00	6985.0
70.00	527.0
72.00	370.0
73.00	3260.0
74.10	11006.0
75.00	35784.0
76.00	3083.0
77.00	497.0
78.00	345.0
79.00	2012.0
79.90	590.0
80.90	2210.0
81.90	472.0
82.90	97.0
86.00	84.0
87.00	3452.0
87.90	3046.0
90.90	176.0
92.00	2015.0
93.00	3339.0
94.10	8372.0
95.00	72520.0
96.00	4930.0
97.10	165.0
103.00	137.0
103.90	276.0
105.00	181.0
105.90	368.0
106.90	87.0
109.60	63.0
113.00	83.0
114.80	73.0
115.20	52.0
115.90	233.0
117.00	452.0
118.00	220.0
118.90	499.0
124.90	145.0
125.80	105.0
127.80	244.0
128.90	141.0
129.90	181.0
130.90	75.0
133.00	441.0
134.90	138.0
137.00	123.0
140.90	633.0
142.90	602.0
143.80	81.0
144.90	144.0
145.80	117.0
147.90	148.0
148.80	101.0
149.90	70.0
154.80	206.0
157.10	102.0
158.90	122.0
160.90	185.0
171.90	282.0
173.90	51672.0
174.90	4231.0
175.90	54448.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

176.90	3701.0
178.00	139.0
179.10	108.0
191.00	470.0
191.90	117.0
193.00	649.0
194.10	54.0
194.80	147.0
205.00	136.0
206.80	321.0
207.90	88.0
248.80	453.0
250.00	145.0
251.00	198.0
265.00	377.0
266.00	131.0
267.10	54.0
281.00	6823.0
282.00	1818.0
283.00	1230.0
284.00	272.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

m/z	Abundance
36.00	451.0
37.00	2566.0
38.10	2192.0
39.00	1002.0
40.00	177.0
44.00	378.0
45.10	561.0
46.10	64.0
47.00	660.0
48.00	470.0
49.10	2613.0
50.00	12327.0
51.00	3904.0
51.90	202.0
55.00	137.0
56.10	905.0
57.10	1783.0
58.00	91.0
58.90	82.0
60.10	656.0
61.00	3143.0
62.00	3209.0
63.00	2489.0
64.10	256.0
65.00	247.0
66.10	52.0
67.00	223.0
68.00	6956.0
69.00	7571.0
70.00	655.0
71.90	302.0
73.00	3162.0
74.00	11811.0
75.10	34992.0
76.00	3076.0
76.90	361.0
77.90	370.0
78.90	2087.0
79.90	576.0
80.90	2200.0
81.90	459.0
83.00	76.0
86.10	77.0
87.00	3191.0
88.00	3240.0
90.90	237.0
92.00	2163.0
93.00	3068.0
94.00	8860.0
95.10	73696.0
96.00	4969.0
97.00	176.0
103.00	90.0
103.90	379.0
105.00	125.0
105.90	266.0
106.80	104.0
111.00	51.0
112.90	72.0
114.80	61.0
115.90	230.0
116.90	473.0
117.90	262.0
118.90	415.0
123.70	58.0
125.80	76.0
127.00	53.0
127.80	185.0
128.80	123.0
129.90	317.0
131.00	118.0
132.90	239.0
134.90	137.0
137.00	114.0
140.90	751.0
141.80	51.0
143.00	830.0
143.80	62.0
145.10	130.0
145.90	102.0
147.90	205.0
150.10	73.0
154.90	202.0
155.90	63.0
157.00	178.0
158.80	87.0
161.00	152.0
171.90	364.0
172.90	613.0
173.90	69424.0
175.00	4506.0
176.00	69152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

177.00	4241.0
178.00	175.0
191.00	302.0
191.90	67.0
193.00	224.0
206.90	125.0
248.90	205.0
249.80	61.0
250.90	116.0
265.00	251.0
267.20	96.0
281.10	3538.0
282.10	796.0
283.00	648.0
284.00	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

m/z	Abundance
36.00	343.0
37.10	1814.0
38.10	1468.0
39.00	698.0
40.00	154.0
44.00	367.0
45.00	224.0
47.00	595.0
48.00	289.0
49.10	2000.0
50.00	8345.0
51.10	2541.0
52.00	167.0
55.00	211.0
56.00	735.0
57.00	1100.0
58.00	74.0
60.00	397.0
61.00	2339.0
62.00	2590.0
63.00	1691.0
64.10	212.0
65.10	226.0
67.10	104.0
68.00	4925.0
69.00	5044.0
69.90	421.0
72.00	329.0
73.00	2300.0
74.00	8733.0
75.00	26056.0
76.10	2378.0
76.90	318.0
78.00	203.0
79.00	1603.0
80.00	412.0
80.90	1803.0
82.00	365.0
85.80	81.0
87.00	2323.0
88.00	2402.0
90.90	119.0
92.00	1498.0
93.00	2609.0
94.00	5868.0
95.00	53168.0
96.00	3506.0
97.00	119.0
103.80	273.0
105.00	73.0
105.80	151.0
106.80	52.0
113.00	81.0
116.00	210.0
116.90	415.0
117.90	182.0
118.80	285.0
128.00	263.0
128.90	91.0
129.90	207.0
130.70	89.0
132.90	111.0
134.90	99.0
137.10	103.0
140.90	502.0
143.00	651.0
146.00	96.0
147.80	127.0
149.90	63.0
154.90	157.0
155.90	82.0
156.90	112.0
158.90	112.0
160.80	89.0
172.00	346.0
173.90	53200.0
175.00	4179.0
175.90	50168.0
176.90	3052.0
177.90	166.0
190.90	63.0
192.90	159.0
207.20	66.0
248.90	81.0
265.00	172.0
281.00	1381.0
282.10	373.0
283.00	232.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435