




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
Data File : VW028001.D
Acq On : 14 Feb 2024 13:05
Operator : SY/MD
Sample : P1442-14
Misc : 5.31g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH9S0

Manual IntegrationsAPPROVED

Quant Time: Feb 15 00:30:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 00:29:03 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/15/2024
Supervised By :Mahesh Dadoda 02/17/2024

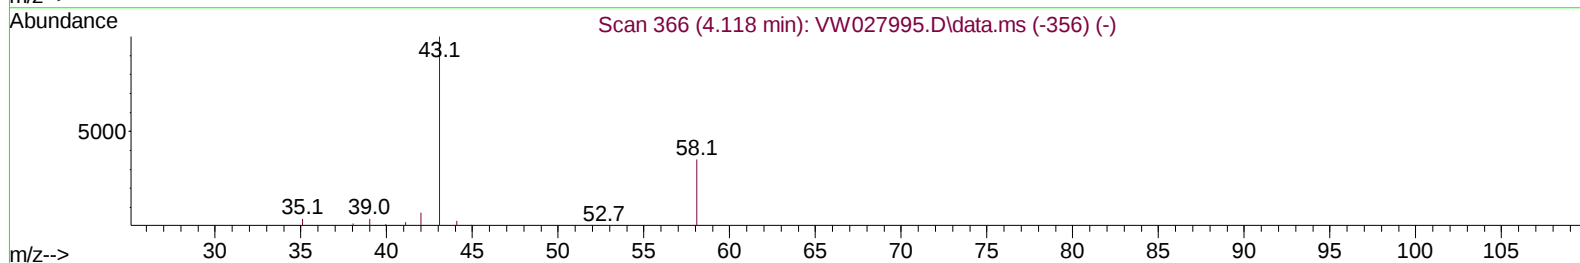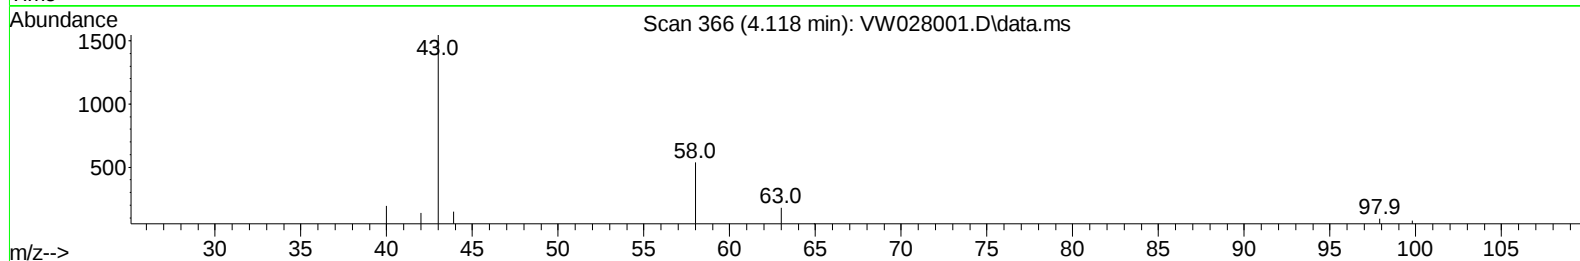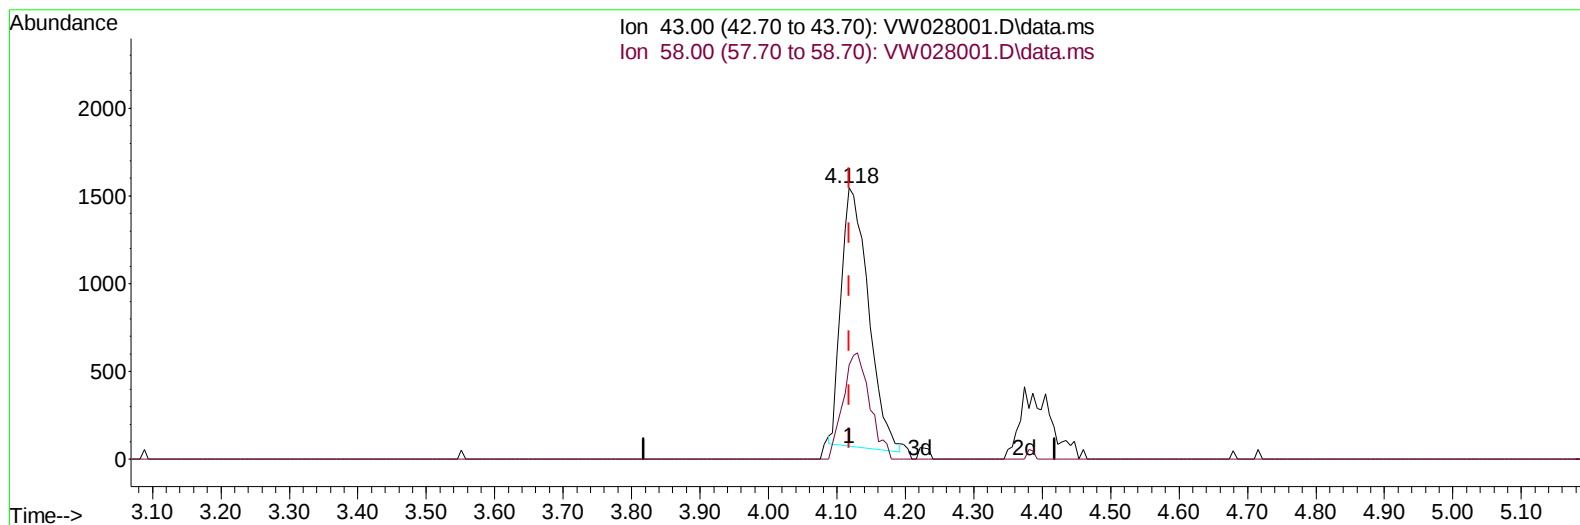

TIC: VW028001.D\data.ms

(13) Acetone (T)

4.118min (-0.000) 7.57 ug/L

response 4042

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.00	38.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
Data File : VW028001.D
Acq On : 14 Feb 2024 13:05
Operator : SY/MD
Sample : P1442-14
Misc : 5.31g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH9S0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/15/2024
Supervised By :Mahesh Dadoda 02/17/2024

Quant Time: Feb 15 00:30:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 00:29:03 2024
Response via : Initial Calibration

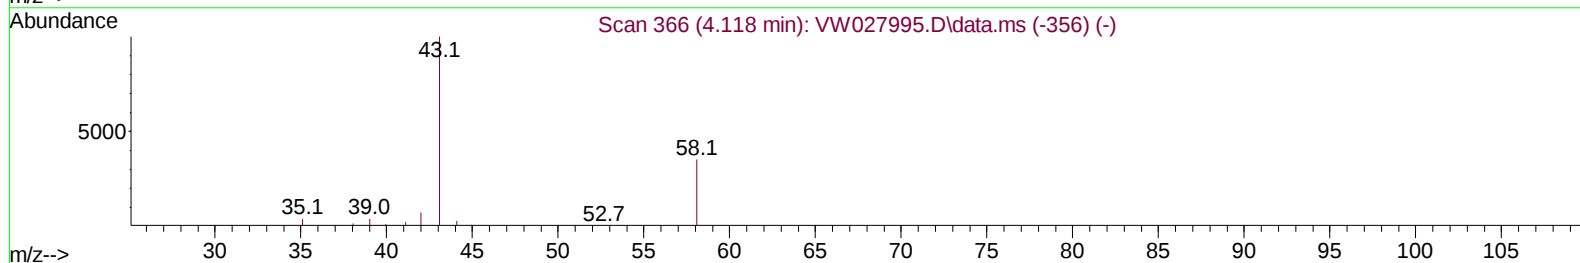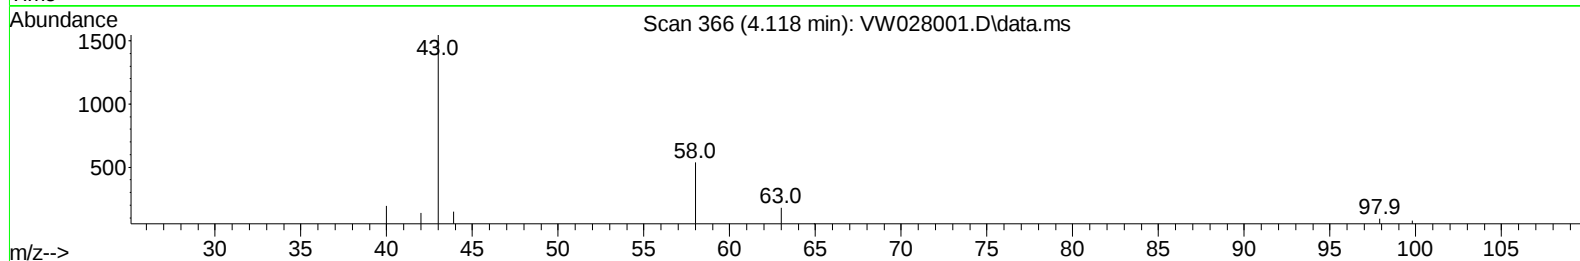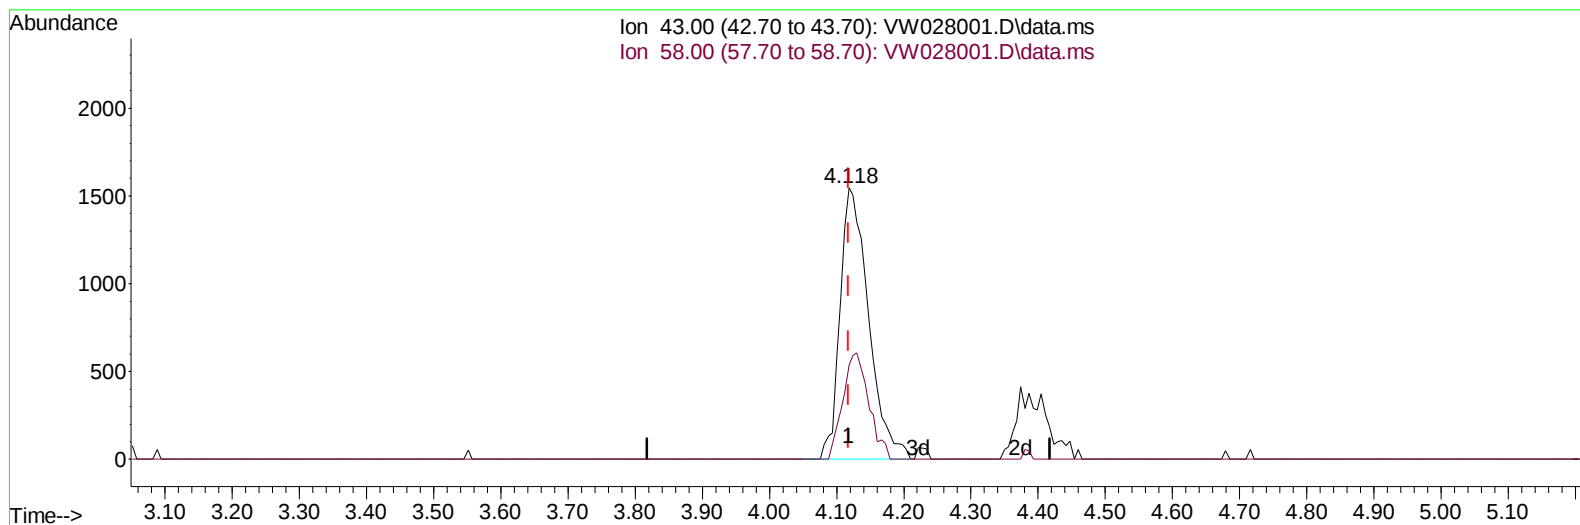

TIC: VW028001.D\data.ms

(13) Acetone (T)

4.118min (-0.000) 8.59 ug/L m

response 4586

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.00	33.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
 Data File : VW028001.D
 Acq On : 14 Feb 2024 13:05
 Operator : SY/MD
 Sample : P1442-14
 Misc : 5.31g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH9S0

Manual IntegrationsAPPROVED

Quant Time: Feb 15 00:30:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 15 00:29:03 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/15/2024
 Supervised By :Mahesh Dadoda 02/17/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	301768	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	262304	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114619	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	61948	17.527	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.120%	
7) Chloroethane-d5	2.899	69	57671	21.513	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.040%	
11) 1,1-Dichloroethene-d2	4.021	65	28850	19.077	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.320%	
21) 2-Butanone-d5	7.075	46	32621	59.400	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	118.800%	
24) Chloroform-d	7.648	84	162216	22.990	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.960%	
26) 1,2-Dichloroethane-d4	8.300	65	82685	25.946	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.800%	
32) Benzene-d6	8.276	84	318440	22.691	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.760%	
36) 1,2-Dichloropropane-d6	9.270	67	93668	24.616	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	98.480%	
41) Toluene-d8	10.318	98	300324	22.366	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.480%	
43) trans-1,3-Dichloroprop...	10.574	79	38771	24.776	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	99.120%	
47) 2-Hexanone-d5	10.922	63	30525	58.977	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	117.960%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	77368	27.204	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152	98192	25.205	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.800%	
Target Compounds						
13) Acetone	4.118	43	4586m	8.588	ug/L	
16) Methylene chloride	4.923	84	8416	2.231	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
Data File : VW028001.D
Acq On : 14 Feb 2024 13:05
Operator : SY/MD
Sample : P1442-14
Misc : 5.31g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH9S0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/15/2024
Supervised By :Mahesh Dadoda 02/17/2024

Quant Time: Feb 15 00:30:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 00:29:03 2024
Response via : Initial Calibration

