

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
 Data File : VW028009.D
 Acq On : 14 Feb 2024 16:16
 Operator : SY/MD
 Sample : P1469-05
 Misc : 5.62g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH9W6

Quant Time: Feb 15 00:32:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 15 00:29:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	386690	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	341583	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	183822	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	76796	16.956	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.840%
7) Chloroethane-d5	2.899	69	72448	21.090	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.360%
11) 1,1-Dichloroethene-d2	4.021	65	35369	18.251	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.000%
21) 2-Butanone-d5	7.081	46	48786	69.326	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	138.660%#
24) Chloroform-d	7.648	84	198662	21.972	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.880%
26) 1,2-Dichloroethane-d4	8.301	65	100916	24.713	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.840%
32) Benzene-d6	8.276	84	399518	21.861	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.440%
36) 1,2-Dichloropropane-d6	9.270	67	112530	22.710	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.840%
41) Toluene-d8	10.319	98	372840	21.322	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.280%
43) trans-1,3-Dichloroprop...	10.575	79	49550	24.316	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.280%
47) 2-Hexanone-d5	10.922	63	46282	68.667	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.340%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	106601	28.783	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.120%
66) 1,2-Dichlorobenzene-d4	13.848	152	147136	23.550	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.200%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	15882	3.286	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
Data File : VW028009.D
Acq On : 14 Feb 2024 16:16
Operator : SY/MD
Sample : P1469-05
Misc : 5.62g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH9W6


Quant Time: Feb 15 00:32:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 00:29:03 2024
Response via : Initial Calibration

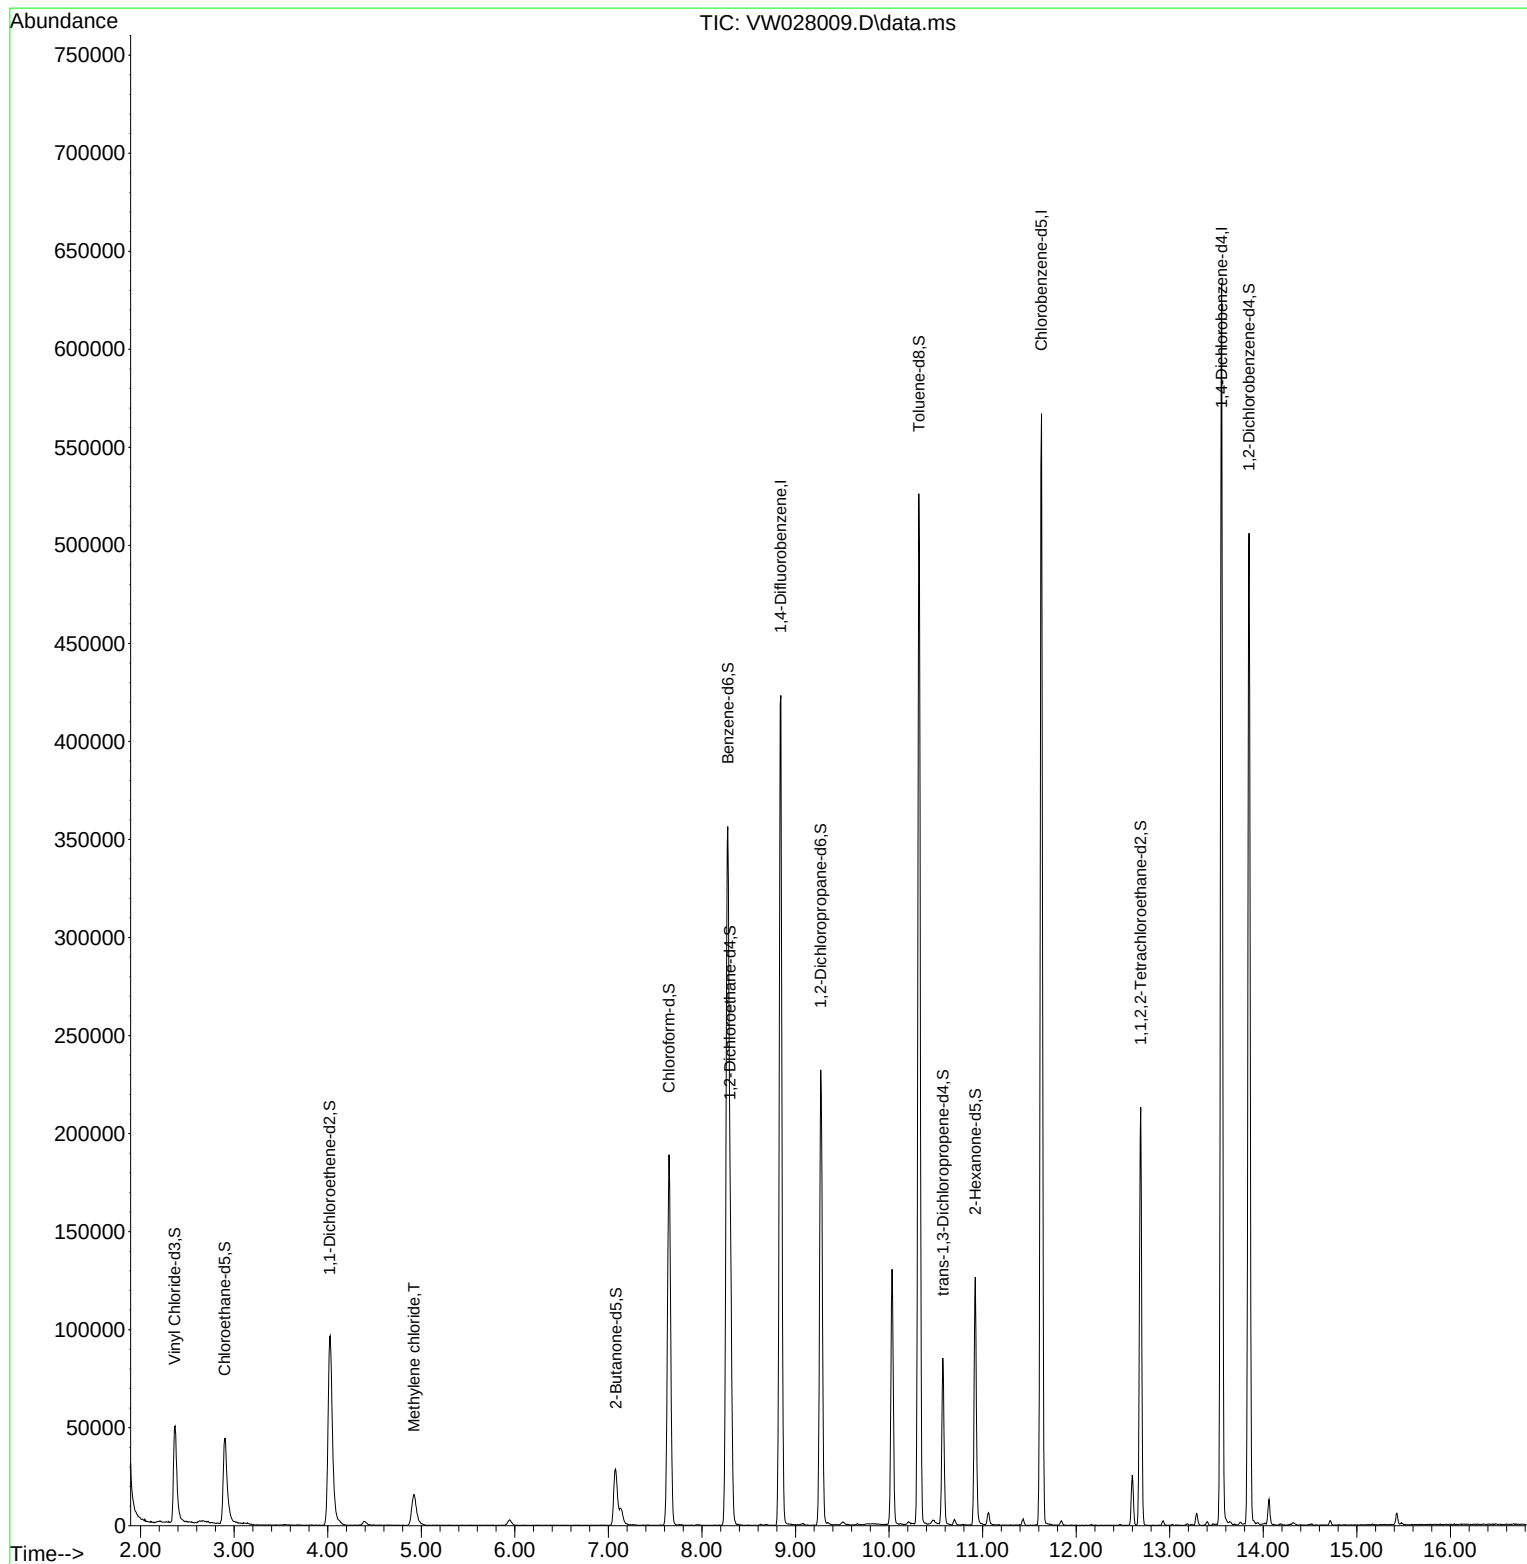

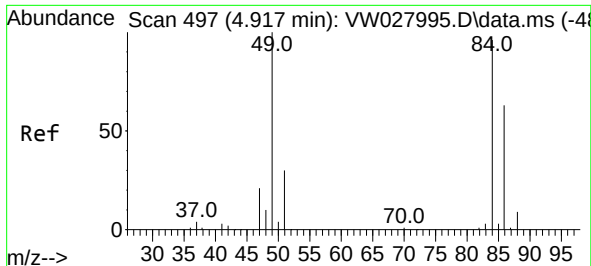

#16
Methylene chloride
Concen: 3.286 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW028009.D
Acq: 14 Feb 2024 16:16

Instrument :
MSVOA_W
ClientSampleId :
BH9W6

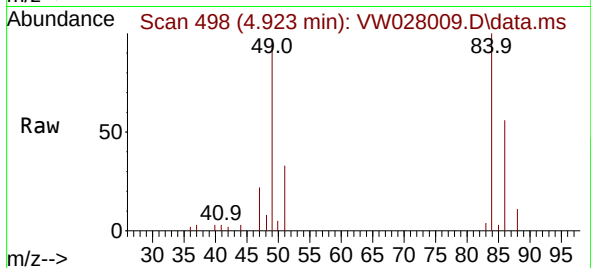

Tgt Ion:	84	Resp:	15882
Ion	Ratio	Lower	Upper
84	100		
86	56.5	45.4	84.4
49	96.5	66.3	123.1

