
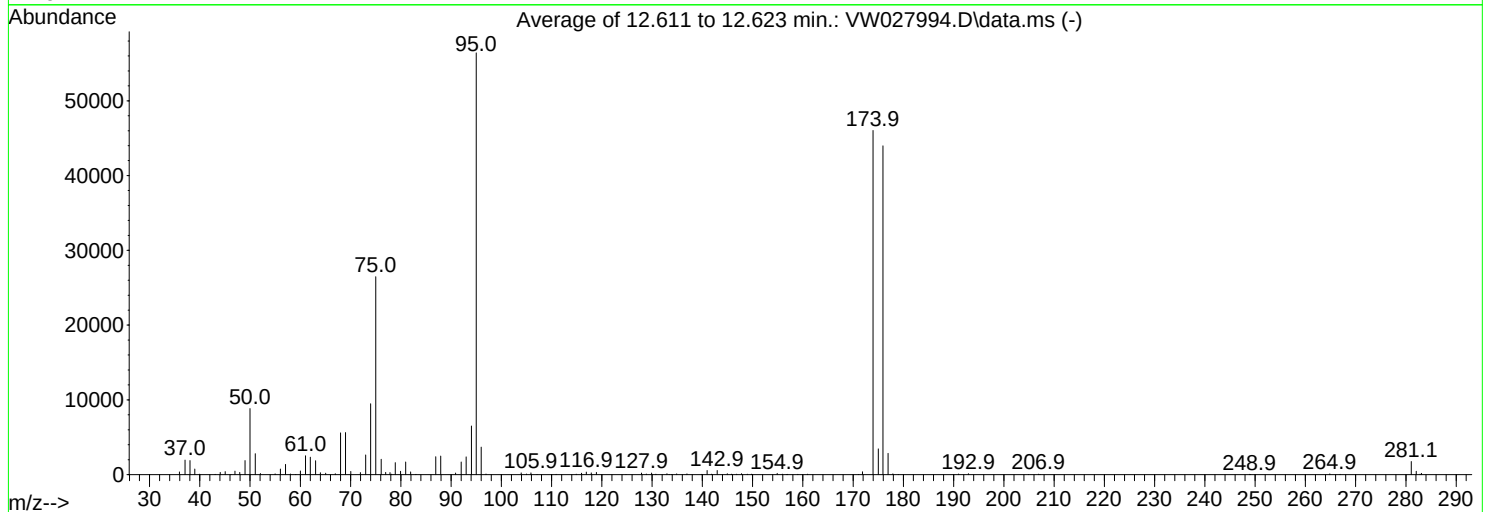


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021424\
Data File : VW027994.D
Acq On : 14 Feb 2024 08:49
Operator : SY/MD
Sample : BFB436
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB436

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Thu Feb 15 00:29:03 2024

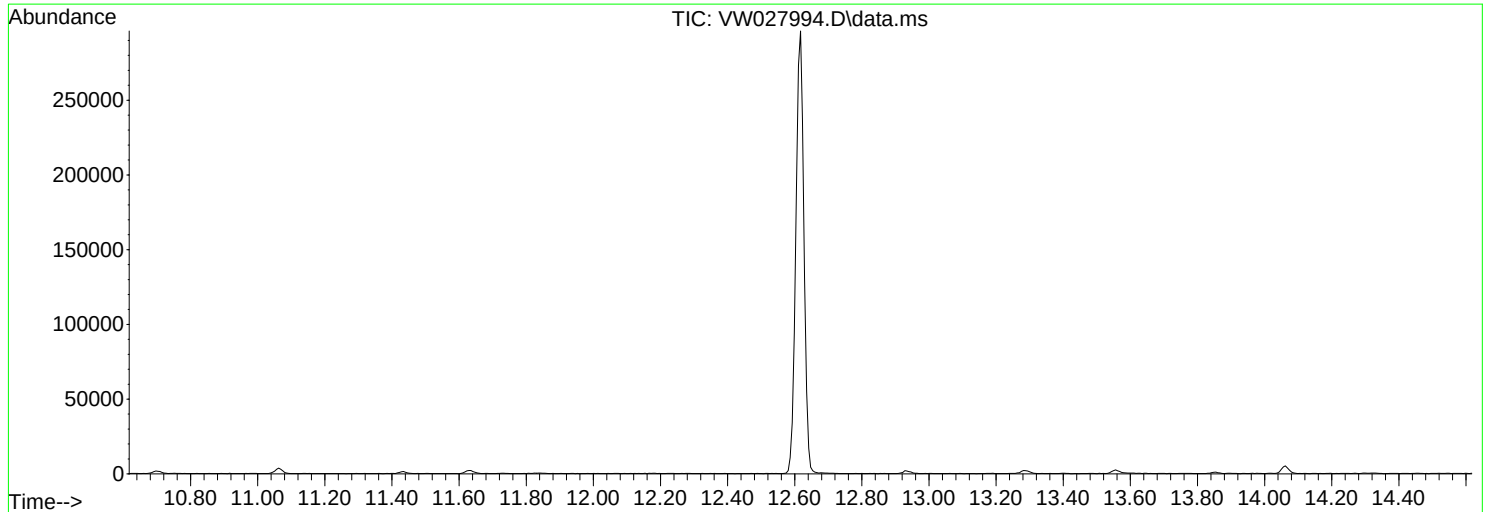

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	8843	PASS
75	95	30	80	46.9	26469	PASS
95	95	100	100	100.0	56416	PASS
96	95	5	9	6.5	3682	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.6	46029	PASS
175	174	5	9	7.5	3436	PASS
176	174	95	101	95.6	43984	PASS
177	176	5	9	6.5	2857	PASS

m/z	Abundance
40.00	106.0
44.10	74.0

Instrument :
MSVOA_W
ClientSampleId :
BFB436

m/z	Abundance
36.00	317.0
37.00	2255.0
38.00	2243.0
39.00	806.0
40.10	149.0
43.10	61.0
44.10	325.0
45.00	492.0
47.00	510.0
47.90	254.0
49.00	2240.0
50.00	10000.0
51.00	3282.0
52.00	141.0
55.00	122.0
56.10	805.0
57.00	1533.0
58.00	120.0
59.10	57.0
60.00	503.0
61.10	2671.0
62.00	2526.0
63.10	1993.0
64.00	320.0
65.10	180.0
66.90	166.0
68.00	6101.0
69.00	5667.0
70.00	499.0
71.90	250.0
73.00	2835.0
74.00	9976.0
75.00	28568.0
76.10	2156.0
77.10	286.0
77.80	191.0
78.10	187.0
78.90	1760.0
79.90	333.0
81.00	1777.0
81.90	271.0
87.00	2712.0
87.90	2592.0
91.00	242.0
92.00	1740.0
93.00	2658.0
94.00	6862.0
95.00	56768.0
96.00	4205.0
97.00	128.0
103.90	360.0
105.00	80.0
105.90	284.0
107.10	65.0
110.00	60.0
110.90	88.0
114.90	88.0
116.00	202.0
116.90	331.0
117.90	173.0
118.90	282.0
124.80	80.0
127.90	231.0
128.80	95.0
129.90	229.0
130.70	93.0
133.00	270.0
133.90	72.0
134.90	115.0
136.90	102.0
139.90	64.0
141.00	407.0
142.00	89.0
142.90	605.0
144.90	114.0
146.90	124.0
147.80	165.0
149.10	68.0
149.80	90.0
155.00	111.0
155.90	57.0
156.70	59.0
161.00	96.0
171.90	411.0
174.00	39768.0
175.00	3349.0
176.00	43288.0
177.00	2872.0
177.90	118.0
179.00	89.0
191.00	128.0
193.00	270.0

Instrument :
MSVOA_W
ClientSampleId :
BFB436

204.90	51.0
206.90	186.0
248.90	120.0
250.00	73.0
264.90	213.0
266.90	111.0
281.00	2936.0
282.10	782.0
283.20	306.0

Instrument :
MSVOA_W
ClientSampleId :
BFB436

m/z	Abundance
35.90	440.0
37.00	2004.0
38.00	1861.0
39.00	816.0
39.90	154.0
43.00	59.0
44.00	453.0
45.10	425.0
46.20	55.0
47.00	572.0
48.00	415.0
49.00	2018.0
50.00	9559.0
51.10	3075.0
52.10	144.0
55.00	111.0
56.00	802.0
57.00	1443.0
58.10	104.0
60.00	511.0
61.00	2972.0
62.00	2416.0
63.00	2003.0
64.00	252.0
65.00	245.0
67.00	151.0
68.00	6064.0
69.00	6360.0
70.10	462.0
72.00	333.0
73.00	2969.0
74.00	10676.0
75.00	28920.0
76.10	2358.0
76.90	361.0
77.90	360.0
78.90	1808.0
80.00	588.0
80.90	1940.0
81.90	514.0
83.00	73.0
86.90	2361.0
87.90	2707.0
90.90	217.0
92.00	1874.0
93.00	2533.0
94.10	6916.0
95.00	64104.0
96.00	3595.0
96.90	125.0
104.00	211.0
105.00	111.0
105.90	237.0
110.90	65.0
114.90	93.0
115.90	214.0
116.90	400.0
117.80	300.0
119.00	375.0
127.90	262.0
128.80	77.0
129.90	192.0
130.80	86.0
132.80	115.0
133.40	51.0
134.90	90.0
136.90	96.0
139.90	51.0
140.90	654.0
141.80	56.0
143.00	633.0
144.90	117.0
145.80	104.0
146.70	51.0
147.80	138.0
148.90	72.0
149.80	82.0
154.80	190.0
156.00	60.0
156.90	97.0
159.00	74.0
160.90	98.0
171.80	436.0
174.00	52312.0
175.00	3897.0
175.90	46800.0
176.90	3290.0
177.90	138.0
191.00	95.0
192.90	109.0
207.20	94.0
249.10	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB436

264.80	145.0
281.10	1562.0
282.00	394.0
283.00	204.0

Instrument :
MSVOA_W
ClientSampleId :
BFB436

m/z	Abundance
36.00	343.0
37.10	1557.0
38.10	1554.0
39.00	640.0
40.00	225.0
44.10	318.0
45.10	318.0
47.10	357.0
47.90	245.0
49.10	1369.0
50.00	6971.0
51.00	2071.0
52.10	142.0
55.00	98.0
56.00	654.0
57.10	1122.0
58.10	60.0
60.00	441.0
61.00	1907.0
62.00	2092.0
63.10	1603.0
64.10	172.0
65.00	164.0
66.90	86.0
68.00	4568.0
69.00	4850.0
70.00	353.0
72.00	279.0
73.00	2071.0
74.00	7812.0
75.00	21920.0
76.10	1649.0
77.00	271.0
77.90	285.0
78.90	1237.0
80.00	399.0
81.00	1384.0
82.00	331.0
83.00	64.0
86.90	2130.0
88.00	2150.0
90.80	182.0
92.00	1444.0
93.00	1969.0
94.00	5726.0
95.00	48376.0
96.00	3247.0
104.00	171.0
105.00	67.0
105.90	195.0
115.90	165.0
116.90	321.0
118.00	210.0
118.80	270.0
127.90	174.0
128.90	120.0
129.90	204.0
134.90	94.0
137.00	128.0
140.90	603.0
141.80	73.0
142.90	463.0
145.00	150.0
145.80	88.0
147.80	108.0
148.80	63.0
155.00	199.0
155.80	53.0
157.00	58.0
159.00	90.0
171.10	52.0
171.90	292.0
173.90	46008.0
175.00	3063.0
176.00	41864.0
176.90	2408.0
177.90	73.0
191.00	51.0
281.10	742.0
282.00	195.0
282.80	169.0

Instrument :
MSVOA_W
ClientSampleId :
BFB436