
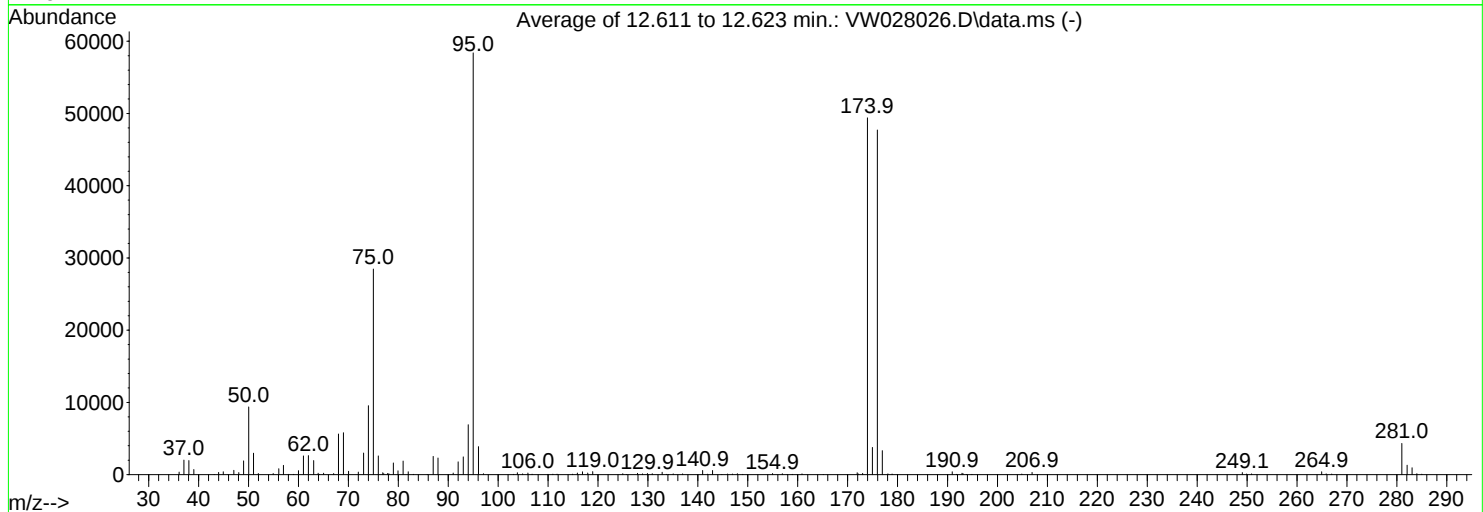


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021624\
Data File : VW028026.D
Acq On : 16 Feb 2024 08:29
Operator : SY/MD
Sample : BFB438
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB438

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Sun Feb 18 23:52:23 2024

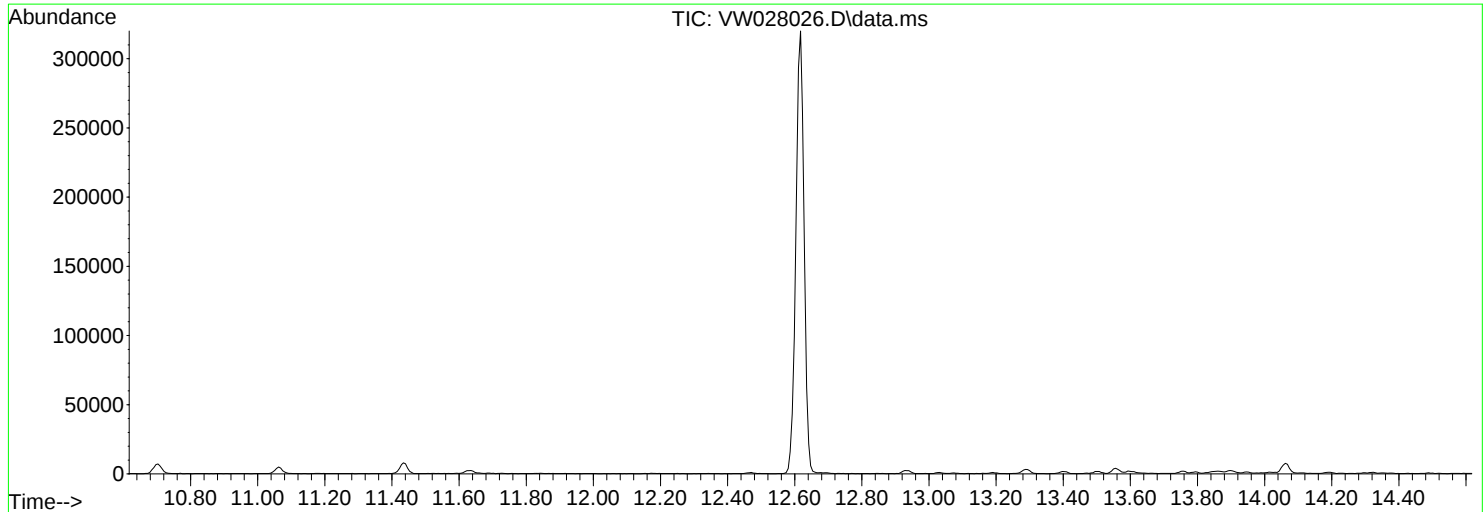

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	9375	PASS
75	95	30	80	48.8	28472	PASS
95	95	100	100	100.0	58392	PASS
96	95	5	9	6.6	3871	PASS
173	174	0.00	2	0.4	181	PASS
174	95	50	120	84.6	49403	PASS
175	174	5	9	7.6	3762	PASS
176	174	95	101	96.6	47707	PASS
177	176	5	9	7.0	3329	PASS

m/z	Abundance
40.00	187.0
44.00	77.0
57.20	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB438

m/z	Abundance
36.10	370.0
37.00	2138.0
38.00	2106.0
39.00	700.0
40.00	147.0
44.00	441.0
44.90	426.0
45.90	55.0
47.10	716.0
48.00	207.0
49.00	1841.0
50.10	10354.0
51.00	3217.0
51.90	142.0
55.00	149.0
56.10	765.0
57.00	1415.0
58.00	88.0
59.10	96.0
60.00	621.0
61.00	2633.0
62.00	2489.0
63.10	2007.0
64.00	261.0
65.00	214.0
67.00	181.0
68.00	5738.0
69.00	5744.0
70.10	385.0
72.00	361.0
73.00	3188.0
74.00	9549.0
75.00	29392.0
76.00	2630.0
76.90	406.0
77.90	352.0
79.00	1693.0
80.00	467.0
81.00	1944.0
82.00	370.0
87.00	2422.0
88.00	2131.0
91.00	229.0
92.00	1684.0
93.00	2323.0
94.00	6927.0
95.00	56904.0
96.00	3930.0
97.10	120.0
103.10	128.0
103.90	315.0
104.80	144.0
106.00	183.0
106.80	52.0
109.90	118.0
110.90	92.0
111.80	72.0
114.90	91.0
115.80	242.0
116.90	318.0
117.90	245.0
118.90	450.0
125.00	295.0
128.00	222.0
128.90	110.0
129.90	197.0
130.90	94.0
132.90	546.0
133.70	163.0
135.10	166.0
136.90	94.0
140.90	408.0
142.00	63.0
142.90	620.0
144.80	87.0
146.00	67.0
146.90	112.0
147.90	176.0
149.00	52.0
155.00	173.0
156.90	137.0
160.90	174.0
165.10	100.0
171.90	428.0
173.00	544.0
173.90	46968.0
175.00	3550.0
175.90	45168.0
176.90	3068.0
178.00	215.0
178.90	141.0
190.90	694.0

Instrument :
MSVOA_W
ClientSampleId :
BFB438

191.80	120.0
192.90	629.0
193.80	73.0
194.90	138.0
204.90	226.0
206.90	487.0
208.10	59.0
249.10	437.0
250.00	111.0
250.90	210.0
265.00	576.0
265.90	187.0
267.00	140.0
281.00	6104.0
282.10	2077.0
283.00	1406.0
284.00	268.0
285.00	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB438

m/z	Abundance
36.10	396.0
37.00	2262.0
38.10	2132.0
39.00	782.0
40.10	134.0
44.00	313.0
45.00	443.0
47.00	542.0
48.10	319.0
49.00	2450.0
50.10	10194.0
51.00	3476.0
52.00	205.0
55.00	225.0
56.10	972.0
57.00	1467.0
58.10	81.0
59.00	73.0
60.00	632.0
61.00	2884.0
62.00	3065.0
63.00	1919.0
63.90	217.0
65.00	198.0
67.00	141.0
68.00	6223.0
69.00	6238.0
70.00	608.0
72.00	384.0
73.10	3241.0
74.00	10749.0
75.00	31416.0
76.00	3117.0
76.90	373.0
78.10	232.0
79.00	1825.0
79.90	592.0
80.90	2290.0
82.00	443.0
83.00	55.0
85.80	51.0
87.00	2797.0
87.90	2616.0
91.00	225.0
92.00	1995.0
93.00	2951.0
94.00	7525.0
95.00	66576.0
96.00	4494.0
97.00	185.0
103.90	297.0
104.90	140.0
105.90	250.0
106.80	81.0
110.00	53.0
111.00	87.0
111.80	124.0
114.80	62.0
115.90	249.0
116.90	491.0
118.00	246.0
118.90	453.0
124.90	114.0
125.70	50.0
127.90	199.0
128.80	123.0
130.00	148.0
130.90	109.0
132.80	320.0
134.10	68.0
135.00	123.0
136.90	83.0
140.90	726.0
141.90	79.0
143.00	614.0
145.90	141.0
147.00	70.0
147.90	147.0
149.00	59.0
154.90	158.0
156.90	166.0
158.90	74.0
160.80	66.0
172.10	364.0
174.00	52552.0
175.00	4185.0
176.00	51216.0
177.00	3651.0
178.10	134.0
178.90	68.0
191.00	371.0
193.10	355.0

Instrument :
MSVOA_W
ClientSampleId :
BFB438

204.80	54.0
207.00	324.0
249.00	268.0
249.80	157.0
250.90	130.0
264.90	485.0
265.80	97.0
266.90	99.0
281.00	4287.0
281.90	1138.0
283.10	952.0
284.00	127.0
285.00	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB438

m/z	Abundance
36.10	309.0
37.10	1647.0
38.00	1631.0
39.10	664.0
40.00	137.0
43.10	59.0
44.10	385.0
45.00	317.0
47.00	568.0
48.00	308.0
49.00	1456.0
50.00	7576.0
51.00	2190.0
51.90	110.0
54.90	126.0
56.00	704.0
57.00	1157.0
60.00	439.0
61.00	2280.0
62.00	2332.0
63.10	1913.0
63.90	137.0
64.20	131.0
65.10	178.0
67.10	115.0
68.00	4901.0
69.00	5426.0
70.00	391.0
72.00	306.0
73.00	2571.0
74.00	8372.0
75.00	24608.0
76.00	2049.0
77.10	376.0
77.80	148.0
78.10	146.0
79.00	1370.0
79.90	520.0
80.90	1445.0
82.00	394.0
83.00	93.0
87.00	2366.0
88.00	2149.0
91.00	192.0
92.00	1617.0
93.00	2100.0
94.00	6308.0
95.00	51696.0
96.10	3188.0
97.00	97.0
103.80	215.0
105.00	80.0
105.90	262.0
106.80	88.0
115.00	77.0
115.80	164.0
116.90	360.0
118.00	203.0
119.00	388.0
127.80	143.0
129.00	99.0
129.80	132.0
130.80	193.0
132.90	132.0
135.00	81.0
137.00	151.0
141.00	584.0
141.90	61.0
142.90	463.0
145.90	61.0
146.80	105.0
148.00	60.0
154.90	139.0
156.90	126.0
157.90	60.0
158.90	51.0
160.90	86.0
171.90	367.0
173.90	48688.0
174.90	3550.0
176.00	46736.0
177.00	3268.0
178.90	62.0
191.10	114.0
193.10	132.0
207.00	136.0
249.00	131.0
265.00	126.0
265.80	72.0
281.00	2588.0
282.10	721.0
283.10	473.0

Instrument :
MSVOA_W
ClientSampleId :
BFB438