
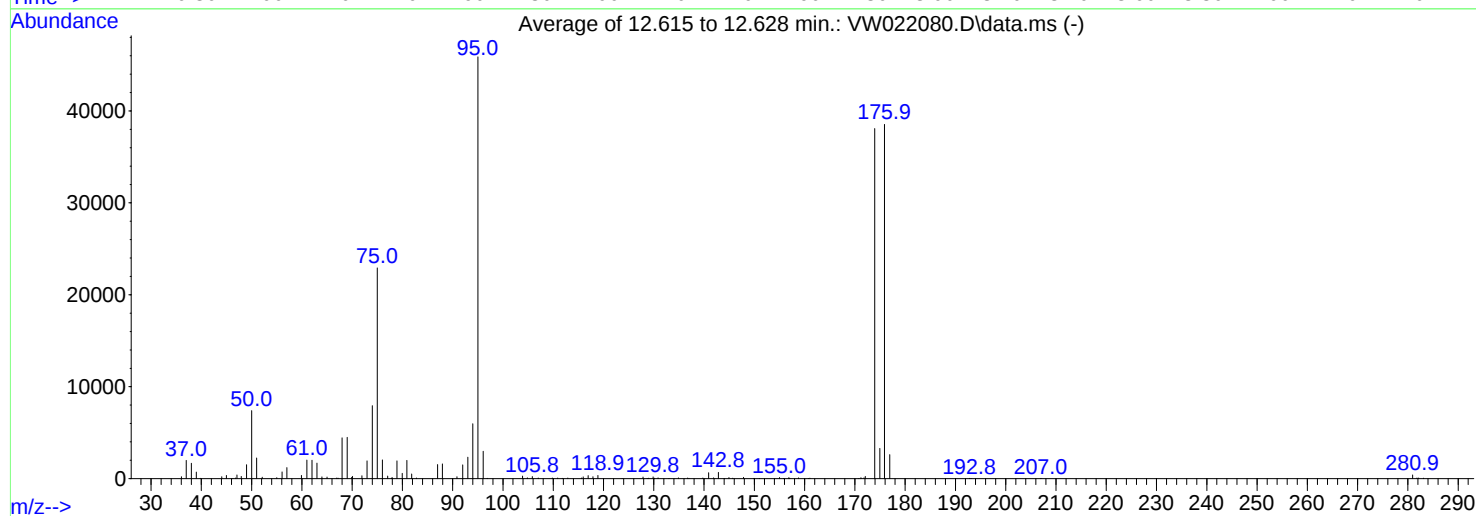


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022122\
 Data File : VW022080.D
 Acq On : 21 Feb 2022 08:53
 Operator : SY/VA
 Sample : BFB510
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB510

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
 Title : SFAM01.0
 Last Update : Tue Feb 22 00:39:16 2022

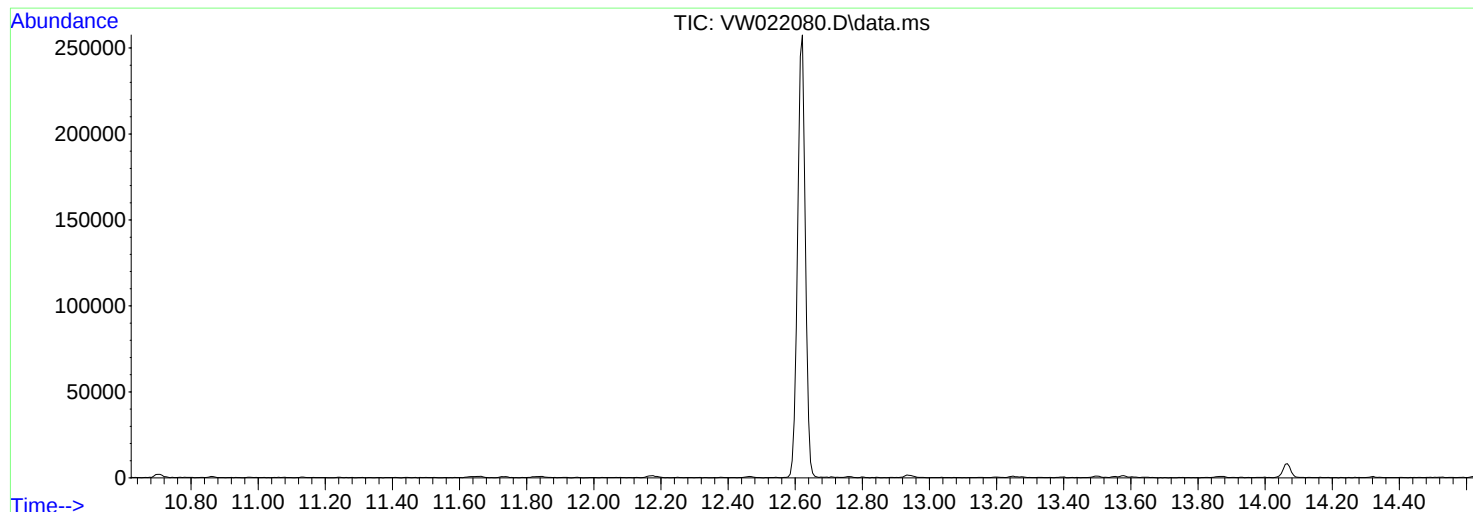

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	7396	PASS
75	95	30	80	50.0	22933	PASS
95	95	100	100	100.0	45885	PASS
96	95	5	9	6.5	2979	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.0	38080	PASS
175	174	5	9	8.6	3282	PASS
176	174	95	105	101.2	38539	PASS
177	176	5	10	6.8	2610	PASS

m/z	Abundance
36.10	71.0
40.00	59.0
40.70	68.0
44.10	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB510

m/z	Abundance
36.00	376.0
37.00	2170.0
38.00	1907.0
39.00	853.0
40.10	83.0
44.00	338.0
45.00	460.0
46.30	77.0
47.10	448.0
48.00	232.0
49.00	1770.0
50.00	8729.0
51.00	2661.0
52.10	203.0
55.00	143.0
56.00	757.0
57.00	1331.0
60.00	437.0
61.00	2399.0
62.00	2420.0
63.00	1876.0
64.00	262.0
65.00	226.0
66.90	132.0
68.00	5003.0
69.00	5140.0
69.90	444.0
72.00	368.0
73.00	2226.0
74.00	9456.0
75.00	25712.0
76.00	2492.0
77.00	358.0
77.80	161.0
78.90	2158.0
80.00	682.0
80.90	2263.0
81.90	608.0
82.80	101.0
87.00	1829.0
87.90	1793.0
90.80	221.0
92.00	1622.0
93.00	2671.0
94.00	6334.0
95.00	51600.0
96.00	3483.0
103.90	367.0
104.90	107.0
105.90	244.0
107.00	91.0
109.80	101.0
110.90	88.0
112.90	79.0
115.90	223.0
117.00	365.0
117.90	212.0
118.90	399.0
123.70	51.0
127.90	137.0
128.70	75.0
129.90	285.0
130.80	104.0
135.00	144.0
136.70	91.0
139.80	60.0
140.90	706.0
141.90	77.0
142.90	839.0
144.00	82.0
145.00	106.0
145.70	61.0
147.80	154.0
155.00	96.0
155.80	65.0
156.90	236.0
158.80	60.0
161.10	54.0
171.20	173.0
172.00	348.0
174.00	36712.0
174.90	3086.0
175.90	37888.0
176.90	2955.0
192.80	101.0
207.00	102.0
280.90	597.0
281.80	204.0
283.10	176.0

Instrument :
MSVOA_W
ClientSampleId :
BFB510

m/z	Abundance
36.10	276.0
37.00	2398.0
38.00	2093.0
39.00	863.0
40.00	83.0
44.10	345.0
45.00	358.0
47.00	545.0
47.90	265.0
49.00	1657.0
50.00	8377.0
51.00	2436.0
52.10	158.0
55.10	93.0
56.10	818.0
57.00	1435.0
59.90	334.0
61.00	2331.0
62.00	2214.0
63.00	1961.0
64.00	193.0
64.90	195.0
67.20	164.0
68.00	4971.0
69.00	5215.0
70.10	422.0
71.90	329.0
72.90	2189.0
74.00	8770.0
75.00	25696.0
76.00	2138.0
77.10	289.0
78.00	187.0
78.90	2156.0
79.90	577.0
80.90	2114.0
81.80	525.0
82.80	59.0
86.90	1730.0
88.00	1843.0
90.90	196.0
92.00	1841.0
93.00	2551.0
94.00	7013.0
95.00	51736.0
96.10	3005.0
96.90	62.0
103.80	248.0
104.80	86.0
105.80	280.0
107.00	69.0
109.80	95.0
110.90	133.0
111.80	65.0
112.90	149.0
115.60	186.0
115.90	176.0
116.90	335.0
117.90	285.0
118.90	334.0
127.90	246.0
129.00	69.0
129.80	146.0
130.90	72.0
133.00	56.0
134.80	146.0
136.80	115.0
139.70	89.0
140.90	692.0
141.90	87.0
142.80	638.0
145.00	130.0
145.80	56.0
147.90	136.0
149.90	76.0
151.00	55.0
154.90	174.0
156.80	94.0
157.10	94.0
158.80	159.0
160.80	50.0
161.10	51.0
170.80	73.0
172.10	382.0
173.90	44168.0
175.00	3888.0
175.90	44624.0
177.00	2754.0
193.10	82.0
281.00	406.0
282.10	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB510

m/z	Abundance
36.10	200.0
37.00	1368.0
38.10	1028.0
39.00	448.0
39.80	115.0
44.00	196.0
45.10	247.0
46.80	204.0
47.20	229.0
47.90	234.0
49.00	1140.0
50.00	5083.0
51.00	1668.0
52.00	100.0
54.90	84.0
56.00	644.0
57.00	861.0
59.80	256.0
61.00	1349.0
62.00	1395.0
63.00	1236.0
64.00	135.0
65.10	107.0
67.00	89.0
68.00	3355.0
69.00	3114.0
70.00	291.0
71.90	245.0
73.00	1389.0
74.00	5576.0
75.00	17392.0
76.10	1487.0
77.00	208.0
77.90	183.0
78.90	1467.0
79.90	466.0
80.90	1584.0
81.90	394.0
82.80	73.0
87.10	1058.0
88.00	1180.0
90.90	188.0
92.00	1042.0
93.00	1798.0
94.00	4584.0
95.00	34320.0
96.00	2448.0
96.80	56.0
104.00	210.0
104.80	77.0
105.80	141.0
107.00	57.0
111.80	57.0
116.00	161.0
116.90	295.0
117.90	114.0
118.90	318.0
127.80	134.0
129.00	68.0
129.80	163.0
130.10	163.0
130.90	88.0
137.00	118.0
139.80	50.0
140.90	527.0
141.90	109.0
142.90	583.0
144.80	124.0
145.60	56.0
147.80	119.0
149.90	60.0
155.10	116.0
157.00	67.0
158.90	59.0
161.00	65.0
171.20	130.0
171.80	255.0
173.90	33360.0
175.00	2873.0
175.90	33104.0
176.90	2122.0
281.00	197.0
282.20	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB510