
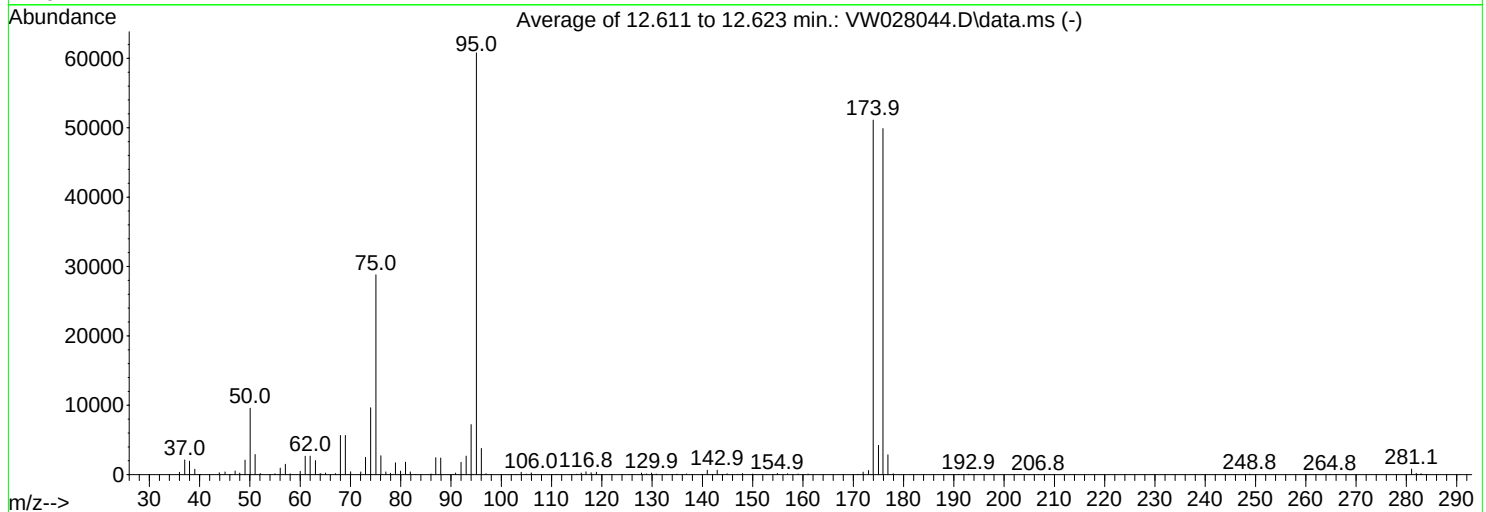


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022124\
Data File : VW028044.D
Acq On : 21 Feb 2024 08:32
Operator : SY/MD
Sample : BFB440
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB440

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Wed Feb 21 23:34:58 2024

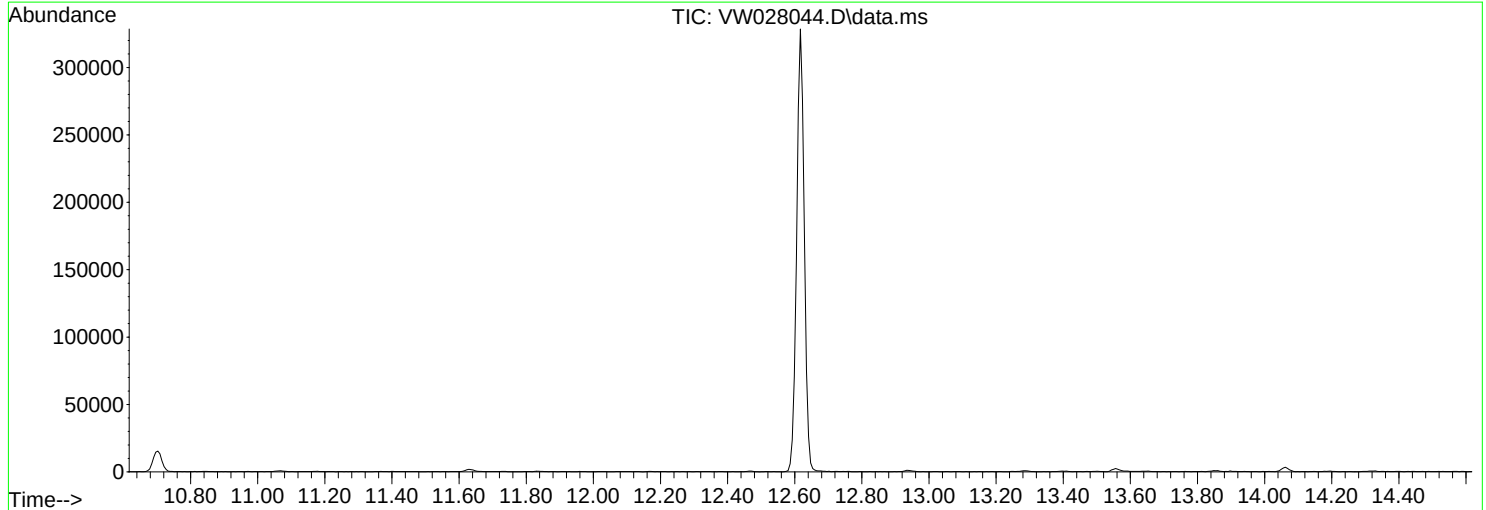

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	9564	PASS
75	95	30	80	47.4	28800	PASS
95	95	100	100	100.0	60795	PASS
96	95	5	9	6.2	3793	PASS
173	174	0.00	2	1.2	597	PASS
174	95	50	120	84.1	51109	PASS
175	174	5	9	8.3	4230	PASS
176	174	95	101	97.6	49880	PASS
177	176	5	9	5.7	2851	PASS

m/z	Abundance
40.00	129.0
43.80	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB440

m/z	Abundance
36.00	347.0
37.00	2243.0
38.00	2103.0
39.00	890.0
40.00	126.0
43.90	368.0
45.00	395.0
47.00	564.0
48.00	237.0
49.00	2317.0
50.10	9344.0
51.00	2840.0
52.10	151.0
55.00	174.0
56.10	943.0
57.00	1602.0
58.00	93.0
60.00	437.0
61.00	2618.0
62.00	2566.0
63.00	2054.0
64.00	269.0
65.00	257.0
67.00	213.0
68.00	5914.0
69.00	5528.0
70.10	376.0
72.00	370.0
73.00	2441.0
74.00	9276.0
75.10	26432.0
76.00	2684.0
77.10	512.0
78.00	204.0
78.90	1625.0
80.00	539.0
81.00	1753.0
81.90	454.0
83.00	61.0
86.00	70.0
86.90	2336.0
88.00	2373.0
90.90	283.0
92.00	1680.0
93.00	2381.0
94.00	6468.0
95.10	56808.0
96.10	3534.0
96.90	159.0
102.90	58.0
104.00	390.0
104.90	77.0
106.00	258.0
110.80	56.0
115.00	71.0
115.90	182.0
117.00	421.0
117.90	221.0
118.90	333.0
127.90	208.0
128.90	59.0
129.90	190.0
130.90	108.0
132.90	115.0
134.80	122.0
136.90	95.0
141.00	589.0
143.00	651.0
144.80	106.0
146.90	84.0
148.00	173.0
150.10	98.0
154.90	171.0
156.90	128.0
159.00	88.0
161.00	63.0
170.90	72.0
172.00	338.0
173.00	484.0
173.90	48240.0
175.00	3710.0
175.90	39064.0
176.90	2905.0
177.90	150.0
190.90	84.0
193.00	113.0
206.80	60.0
248.90	102.0
264.80	99.0
281.00	1137.0
282.00	291.0
282.80	254.0

Instrument :
MSVOA_W
ClientSampleId :
BFB440

m/z	Abundance
36.00	411.0
37.10	2391.0
38.00	1997.0
39.10	839.0
40.10	101.0
44.00	315.0
45.10	434.0
46.30	87.0
47.10	609.0
48.10	279.0
49.10	2217.0
50.00	10969.0
51.10	3207.0
52.00	236.0
55.10	148.0
56.00	1084.0
57.00	1697.0
58.00	137.0
60.00	489.0
61.00	2923.0
62.00	3214.0
63.10	2421.0
64.00	246.0
65.10	242.0
67.00	148.0
68.00	5886.0
69.00	6214.0
70.10	496.0
72.10	410.0
73.00	2833.0
74.00	11011.0
75.00	33832.0
76.10	2845.0
77.00	373.0
77.90	151.0
79.00	1957.0
80.00	539.0
80.90	1960.0
81.90	398.0
86.00	77.0
87.00	2813.0
87.90	2622.0
90.90	221.0
92.00	1761.0
93.00	2924.0
94.00	8536.0
95.00	69416.0
96.00	4408.0
96.90	129.0
103.90	379.0
105.00	123.0
105.80	266.0
106.80	55.0
110.90	53.0
111.90	55.0
114.90	71.0
115.90	262.0
116.80	365.0
117.80	354.0
118.90	358.0
127.90	238.0
128.90	206.0
129.90	270.0
130.70	95.0
135.00	107.0
136.90	142.0
140.90	724.0
142.00	79.0
143.00	718.0
144.90	235.0
146.90	62.0
147.80	163.0
149.90	90.0
154.90	160.0
157.00	130.0
159.10	84.0
161.10	94.0
170.90	92.0
172.00	361.0
173.10	625.0
173.90	56000.0
175.00	4824.0
175.90	57192.0
176.90	2934.0
178.00	193.0
191.00	84.0
192.90	98.0
206.80	64.0
248.80	105.0
281.10	937.0
281.80	137.0
282.20	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB440

283.00

176.0

Instrument :
MSVOA_W
ClientSampleId :
BFB440

m/z	Abundance
36.00	293.0
37.00	1727.0
38.00	1736.0
39.00	632.0
40.00	174.0
44.00	336.0
45.10	316.0
46.10	64.0
47.10	434.0
47.90	210.0
49.00	1764.0
50.00	8378.0
51.10	2676.0
52.10	88.0
54.90	93.0
56.10	835.0
57.10	1222.0
58.00	109.0
60.00	512.0
61.00	2403.0
62.00	2228.0
63.00	1612.0
64.20	189.0
65.00	209.0
67.00	109.0
68.00	5135.0
69.00	5204.0
70.00	358.0
72.00	389.0
73.00	2219.0
74.00	8660.0
75.00	26136.0
76.10	2630.0
77.00	309.0
77.90	262.0
79.00	1571.0
79.90	453.0
81.00	1659.0
81.90	321.0
86.10	109.0
87.00	2203.0
88.00	2230.0
90.90	189.0
92.00	1870.0
93.00	2713.0
94.00	6686.0
95.00	56160.0
96.10	3437.0
97.00	106.0
102.90	56.0
103.90	288.0
105.00	112.0
106.00	251.0
106.90	50.0
110.90	52.0
111.90	56.0
114.90	61.0
115.90	282.0
116.80	444.0
117.90	277.0
118.90	321.0
127.90	249.0
128.90	78.0
129.90	267.0
130.80	101.0
134.90	128.0
136.80	126.0
141.00	624.0
142.90	578.0
145.00	110.0
148.00	168.0
149.80	76.0
152.80	76.0
154.90	199.0
156.90	172.0
159.10	88.0
160.90	89.0
171.90	381.0
173.00	683.0
174.00	49088.0
175.00	4156.0
175.90	53384.0
176.90	2715.0
178.00	104.0
281.00	356.0
281.90	113.0
283.00	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB440