
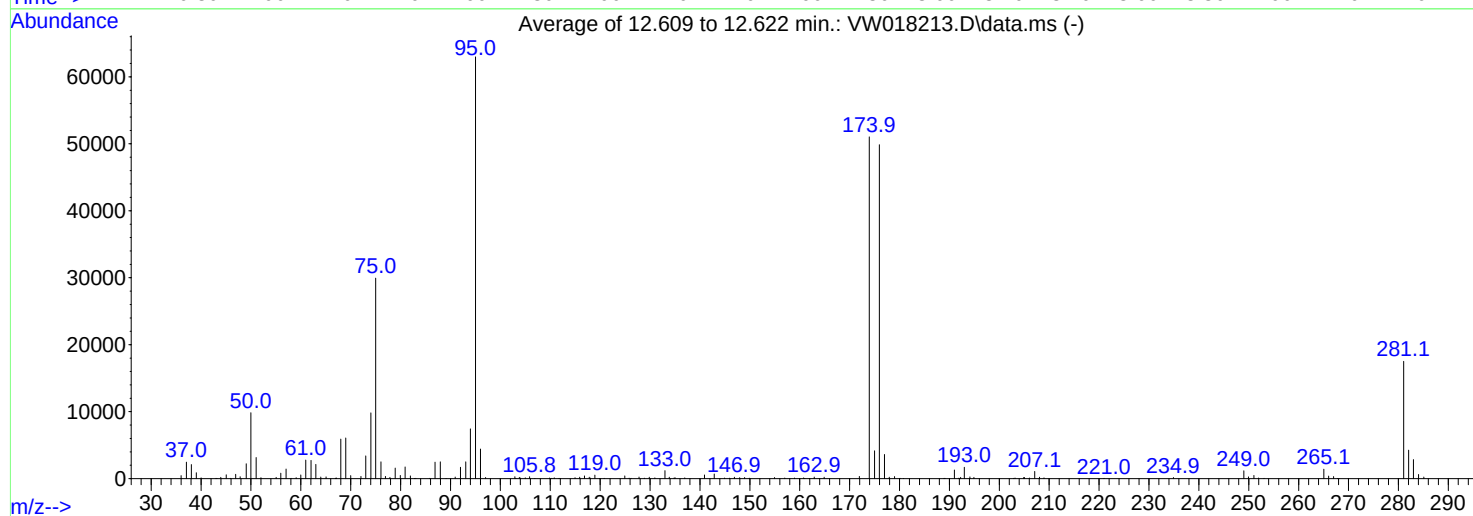


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022221\
 Data File : VW018213.D
 Acq On : 22 Feb 2021 09:30
 Operator : SY/VA
 Sample : BFB09
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB09

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM022221S.M
 Title : VOC Analysis
 Last Update : Tue Feb 23 01:10:51 2021

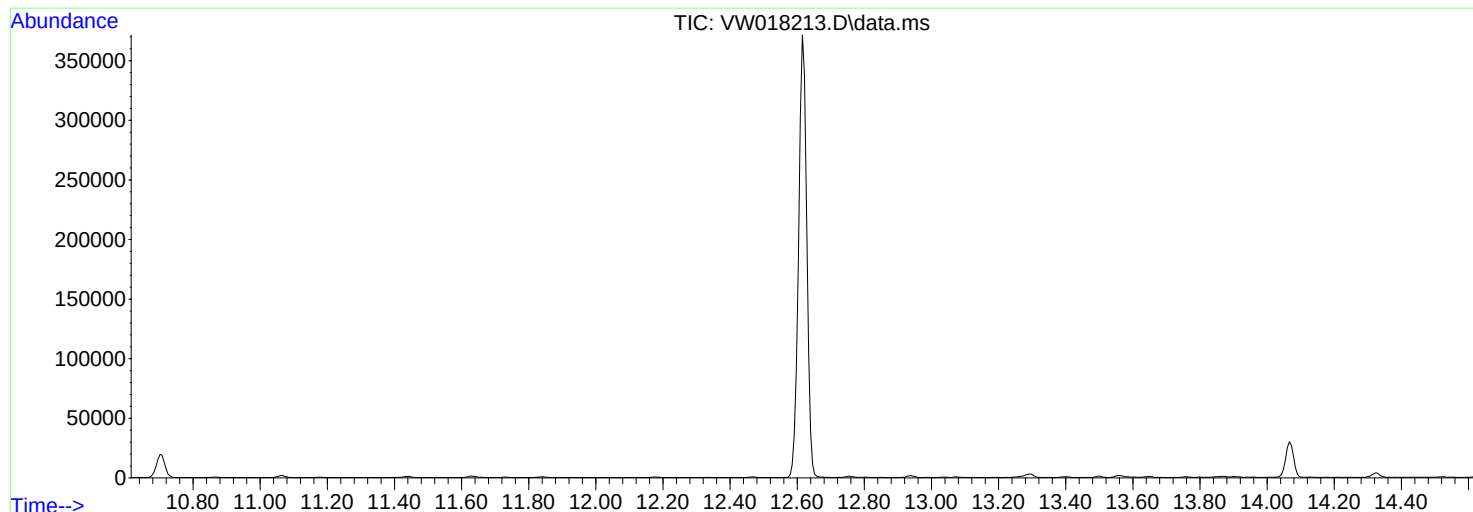

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9840	PASS
75	95	30	80	47.5	29931	PASS
95	95	100	100	100.0	62989	PASS
96	95	5	9	7.0	4418	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.0	51029	PASS
175	174	5	9	8.1	4155	PASS
176	174	95	101	97.7	49856	PASS
177	176	5	9	7.2	3602	PASS

m/z	Abundance
36.00	399.0
37.10	2280.0
38.00	2023.0
39.00	840.0
39.80	139.0
43.00	105.0
44.00	464.0
45.00	623.0
45.90	58.0
46.90	624.0
47.90	224.0
49.00	2092.0
50.00	8913.0
51.00	2778.0
52.00	136.0
55.00	190.0
56.00	676.0
57.10	1486.0
58.00	52.0
59.10	213.0
60.10	407.0
61.00	2285.0
62.10	2267.0
63.00	1991.0
64.00	237.0
65.00	231.0
66.90	88.0
67.20	97.0
68.00	5344.0
69.00	5510.0
70.00	382.0
72.10	346.0
73.00	3546.0
74.00	8648.0
75.00	27184.0
76.00	2284.0
77.00	212.0
78.90	1305.0
79.90	428.0
80.90	1529.0
81.90	396.0
82.80	51.0
85.80	81.0
86.90	1910.0
88.00	2034.0
90.90	234.0
92.00	1476.0
93.10	2256.0
94.00	5948.0
95.00	52768.0
96.00	3950.0
97.00	136.0
103.00	387.0
103.80	326.0
105.10	128.0
105.80	265.0
106.90	52.0
109.80	133.0
110.30	149.0
110.80	175.0
112.00	88.0
115.00	190.0
116.00	194.0
116.90	364.0
117.80	375.0
119.00	555.0
119.90	59.0
120.80	87.0
125.00	452.0
126.20	133.0
127.80	160.0
128.90	94.0
129.90	211.0
131.00	142.0
133.00	1661.0
134.80	297.0
136.90	124.0
141.00	562.0
142.80	469.0
144.90	77.0
146.00	85.0
146.90	263.0
148.00	146.0
149.00	129.0
154.90	144.0
157.00	136.0
159.00	96.0
160.80	176.0
161.90	76.0
163.00	281.0
163.90	53.0
164.90	326.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

172.00	253.0
173.90	39712.0
175.00	3374.0
175.90	39080.0
177.00	2946.0
177.90	176.0
179.00	471.0
180.10	57.0
180.80	55.0
188.90	152.0
191.00	1737.0
192.30	407.0
193.00	2654.0
194.10	424.0
194.90	269.0
203.20	174.0
204.90	495.0
206.00	189.0
207.10	1523.0
208.10	241.0
209.00	186.0
221.00	70.0
234.90	208.0
249.00	1508.0
249.90	412.0
251.10	682.0
252.00	162.0
253.10	60.0
265.10	1946.0
266.00	527.0
267.00	412.0
268.10	83.0
281.00	21592.0
282.00	5594.0
283.00	3644.0
284.00	907.0
285.00	333.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

m/z	Abundance
36.00	542.0
37.10	2672.0
38.00	2465.0
39.00	1000.0
40.00	154.0
43.00	66.0
44.00	477.0
45.00	608.0
45.90	100.0
47.00	691.0
47.90	328.0
49.10	2402.0
50.00	11322.0
51.10	3329.0
52.00	157.0
55.10	189.0
56.00	876.0
57.00	1578.0
58.10	55.0
59.00	150.0
60.00	704.0
61.00	3220.0
62.00	3162.0
63.00	2206.0
63.90	265.0
65.10	311.0
67.00	148.0
68.00	6629.0
69.00	6762.0
70.00	464.0
72.00	417.0
73.00	3494.0
74.10	10916.0
75.00	32920.0
76.00	2795.0
77.00	426.0
77.90	287.0
78.90	1782.0
80.00	535.0
80.90	1861.0
81.90	393.0
83.10	53.0
85.90	104.0
86.90	2982.0
87.90	2581.0
89.10	74.0
90.90	298.0
92.00	2036.0
93.00	2650.0
94.00	8439.0
95.00	69808.0
96.00	4783.0
97.00	200.0
102.80	364.0
104.00	327.0
105.00	169.0
105.90	286.0
109.90	79.0
110.80	141.0
111.70	57.0
114.90	157.0
115.80	235.0
116.80	452.0
118.00	327.0
119.00	504.0
120.80	55.0
124.90	385.0
125.80	191.0
127.70	261.0
128.90	79.0
129.80	240.0
130.90	105.0
133.00	1350.0
133.80	431.0
135.00	282.0
137.00	102.0
140.90	549.0
142.90	814.0
144.90	124.0
145.90	108.0
146.90	238.0
147.90	180.0
148.90	150.0
149.90	79.0
154.90	198.0
156.90	102.0
158.90	118.0
160.80	214.0
162.80	274.0
164.90	203.0
172.00	408.0
173.90	56144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

175.00	4679.0
176.00	54144.0
177.00	4146.0
178.00	250.0
178.90	288.0
180.10	76.0
189.10	102.0
191.00	1336.0
191.90	241.0
193.00	1606.0
194.10	246.0
194.90	220.0
202.90	166.0
205.10	331.0
206.10	98.0
207.10	1039.0
208.00	257.0
208.90	134.0
221.00	54.0
234.90	184.0
249.00	1270.0
250.00	281.0
251.00	518.0
251.90	115.0
253.00	81.0
265.00	1390.0
266.00	394.0
266.90	333.0
267.80	98.0
281.10	19520.0
282.10	4532.0
283.00	3251.0
284.10	646.0
285.10	217.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

m/z	Abundance
36.00	421.0
37.00	2474.0
38.10	1834.0
39.10	813.0
40.00	182.0
43.20	69.0
43.90	447.0
45.10	474.0
47.00	614.0
47.80	305.0
49.00	2141.0
50.00	9285.0
51.00	3330.0
52.00	172.0
55.00	167.0
56.00	866.0
57.00	1228.0
58.10	71.0
59.10	101.0
59.90	576.0
61.00	2821.0
62.00	2725.0
63.00	2168.0
64.10	197.0
65.10	213.0
67.10	174.0
68.00	5718.0
69.00	5910.0
70.00	525.0
72.10	251.0
73.00	3113.0
74.00	9910.0
75.00	29688.0
76.10	2444.0
76.90	366.0
77.80	290.0
78.90	1687.0
80.00	460.0
80.90	1824.0
82.00	428.0
83.00	76.0
86.90	2483.0
88.00	2906.0
91.00	219.0
92.00	1600.0
93.00	2643.0
94.00	7926.0
95.00	66392.0
96.00	4521.0
97.10	176.0
102.70	88.0
103.10	177.0
103.80	282.0
104.90	98.0
105.90	286.0
109.80	58.0
110.70	52.0
111.80	73.0
114.90	122.0
115.90	213.0
116.90	420.0
117.80	290.0
118.90	526.0
125.00	368.0
127.90	267.0
128.80	77.0
129.90	226.0
130.90	138.0
133.10	589.0
133.90	219.0
135.00	192.0
136.90	157.0
140.80	578.0
142.90	814.0
145.00	95.0
146.00	69.0
146.90	125.0
148.00	130.0
148.80	119.0
149.10	110.0
149.90	145.0
155.00	178.0
157.10	95.0
158.90	74.0
161.00	80.0
163.00	161.0
165.00	104.0
171.80	360.0
174.00	57232.0
175.00	4411.0
175.90	56344.0
177.00	3713.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

177.90	214.0
179.10	203.0
189.10	67.0
190.90	783.0
192.10	157.0
193.00	850.0
194.10	113.0
194.80	110.0
203.10	128.0
205.00	180.0
207.10	654.0
208.10	116.0
208.90	83.0
235.00	117.0
248.90	711.0
250.00	107.0
251.10	274.0
265.10	877.0
266.00	241.0
267.10	169.0
281.10	11438.0
282.00	2632.0
283.00	1614.0
284.10	331.0
285.20	140.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

m/z	Abundance
39.90	128.0
44.00	276.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09