

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022223\
 Data File : VW025354.D
 Acq On : 22 Feb 2023 12:38
 Operator : SY/MD
 Sample : VW0222SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK466

Quant Time: Feb 22 21:28:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 22 21:27:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	362289	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	320831	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	153149	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	68607	22.369	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.480%		
7) Chloroethane-d5	2.899	69	52742	23.324	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.280%		
11) 1,1-Dichloroethene-d2	4.027	63	125212	15.728	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.920%		
21) 2-Butanone-d5	7.075	46	35307	50.745	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.500%		
24) Chloroform-d	7.648	84	157552	22.670	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.680%		
26) 1,2-Dichloroethane-d4	8.307	65	86039	23.865	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.480%		
32) Benzene-d6	8.276	84	325571	23.946	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.800%		
36) 1,2-Dichloropropane-d6	9.276	67	91446	23.968	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.880%		
41) Toluene-d8	10.325	98	300595	23.715	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	94.840%		
43) trans-1,3-Dichloroprop...	10.581	79	40884	23.521	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	94.080%		
47) 2-Hexanone-d5	10.922	63	29045	52.188	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.380%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	68984	24.151	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.600%		
66) 1,2-Dichlorobenzene-d4	13.849	152	96092	24.704	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.800%		
Target Compounds					Qvalue	
34) Trichloroethene	8.837	95	11443	2.089	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022223\
Data File : VW025354.D
Acq On : 22 Feb 2023 12:38
Operator : SY/MD
Sample : VW02222SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK466


Quant Time: Feb 22 21:28:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 22 21:27:06 2023
Response via : Initial Calibration

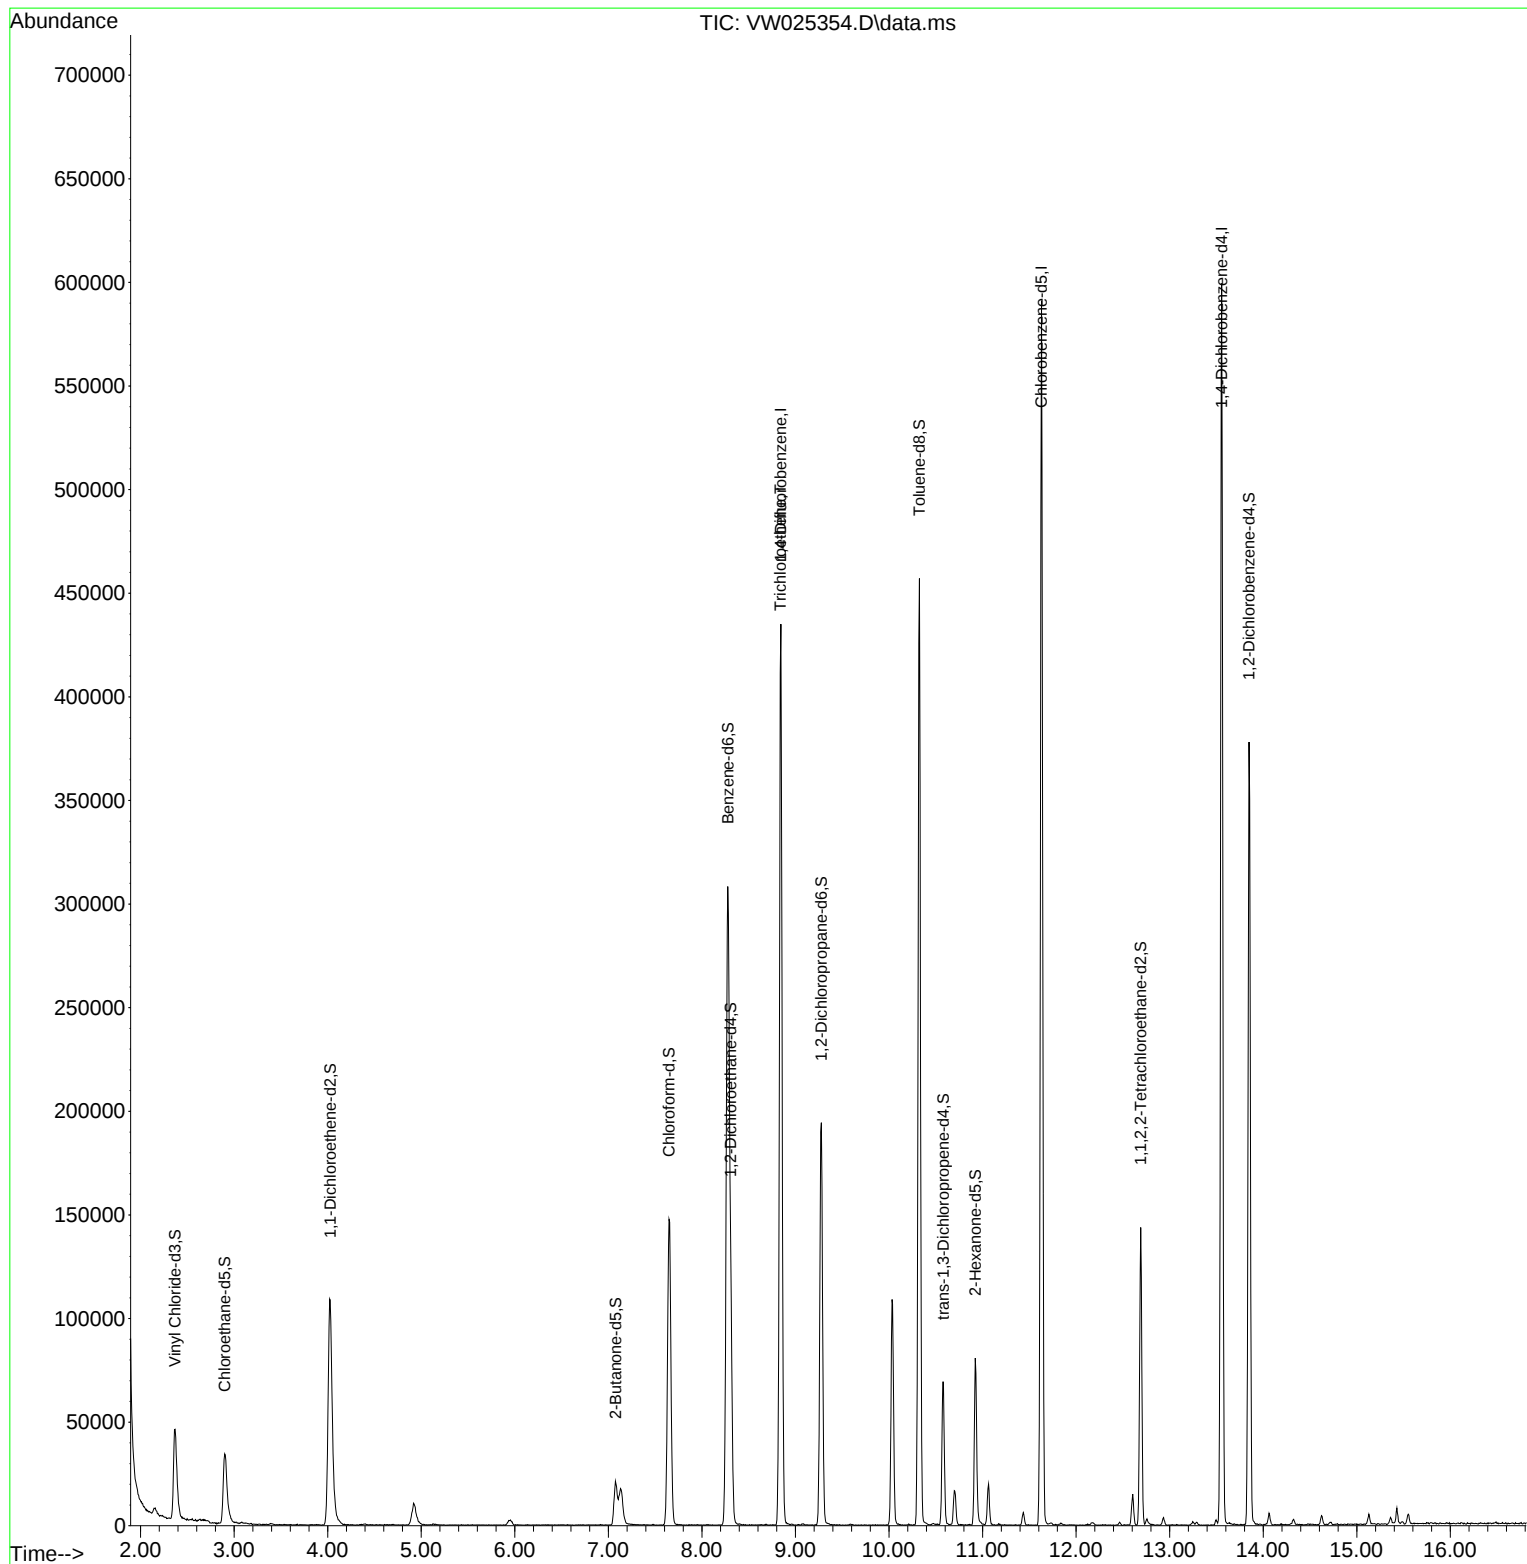

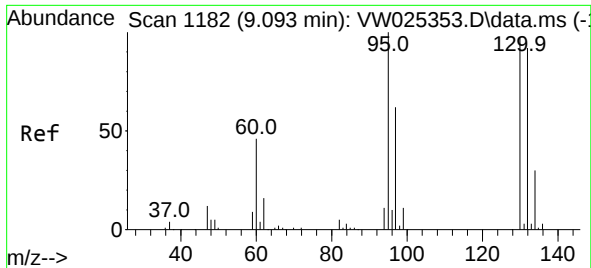

#34
 Trichloroethene
 Concen: 2.089 ug/L
 RT: 8.837 min Scan# 11
 Delta R.T. -0.256 min
 Lab File: VW025354.D
 Acq: 22 Feb 2023 12:38

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK466

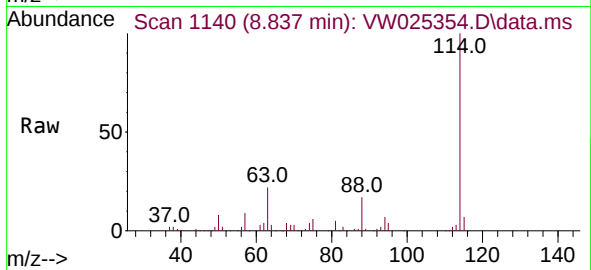

Tgt Ion:	95	Resp:	11443
Ion	Ratio	Lower	Upper
95	100		
97	0.0	46.3	85.9#
132	0.0	69.3	128.7#
130	0.0	72.1	133.9#

