
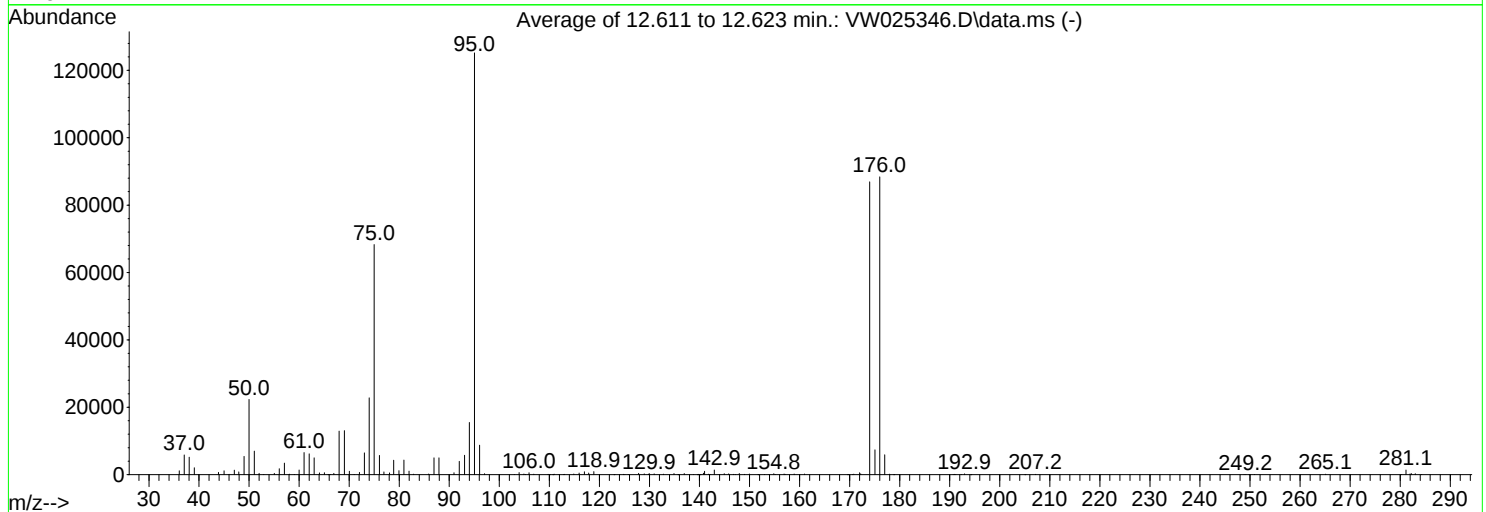


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022223\
Data File : VW025346.D
Acq On : 22 Feb 2023 07:57
Operator : SY/MD
Sample : BFB483
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB483

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
Title : SFAM01.0
Last Update : Wed Feb 22 21:27:06 2023

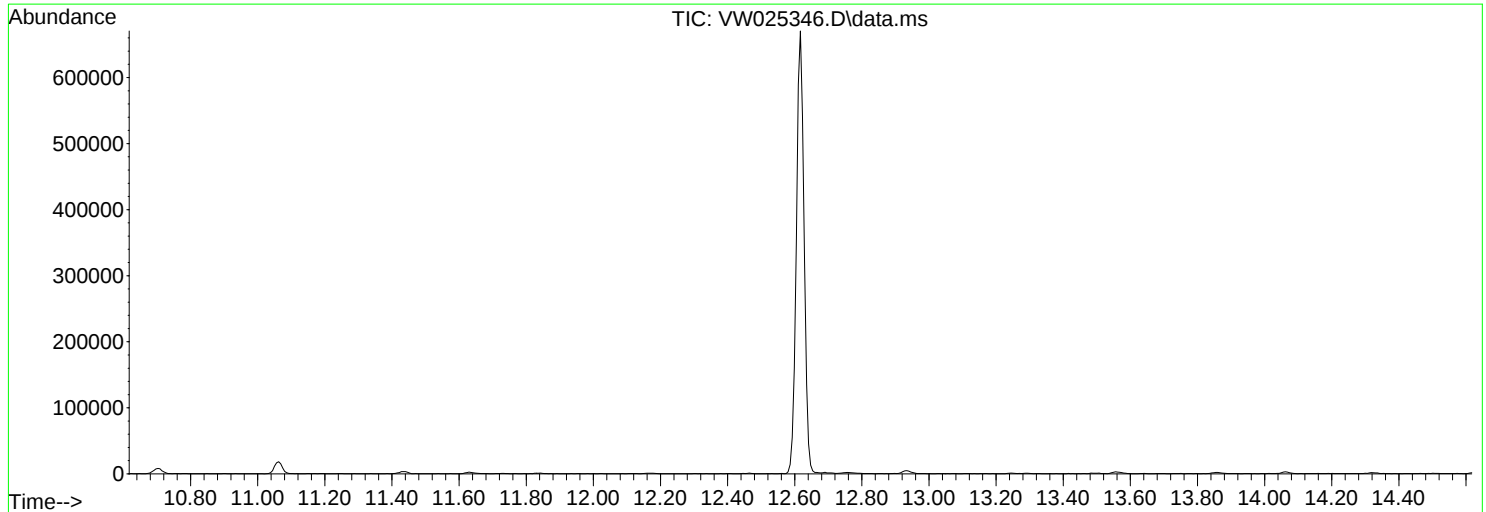

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	22307	PASS
75	95	30	80	54.6	68304	PASS
95	95	100	100	100.0	125203	PASS
96	95	5	9	7.0	8760	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.4	86907	PASS
175	174	5	9	8.5	7348	PASS
176	174	95	105	101.7	88379	PASS
177	176	5	10	6.6	5875	PASS

m/z	Abundance
40.00	214.0
43.20	98.0
43.80	227.0
56.10	88.0
57.20	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

m/z	Abundance
36.10	1219.0
37.00	6389.0
38.10	5238.0
39.00	2210.0
40.00	287.0
43.20	66.0
44.00	932.0
45.00	1183.0
46.00	119.0
47.10	1460.0
48.00	780.0
49.00	5888.0
50.00	23800.0
51.00	7200.0
52.00	481.0
53.00	135.0
55.00	406.0
56.00	1785.0
57.00	3310.0
58.00	123.0
59.00	102.0
60.00	1447.0
61.00	6759.0
62.00	6692.0
63.00	5472.0
64.10	667.0
65.00	733.0
66.10	96.0
67.00	448.0
68.00	13220.0
69.10	13348.0
70.10	1057.0
71.10	52.0
72.00	744.0
73.00	6655.0
74.00	23720.0
75.00	68688.0
76.00	5598.0
76.90	993.0
78.20	414.0
78.90	4618.0
79.90	1152.0
80.90	4671.0
82.00	989.0
82.90	117.0
87.00	4643.0
87.90	4861.0
91.00	548.0
92.00	4124.0
93.00	5834.0
94.00	14684.0
95.10	125896.0
96.10	8872.0
97.10	252.0
104.00	578.0
104.80	90.0
105.20	120.0
106.00	592.0
107.00	139.0
109.80	160.0
110.70	80.0
111.10	75.0
112.00	55.0
113.00	161.0
115.00	211.0
116.00	532.0
117.10	904.0
117.90	552.0
118.90	954.0
124.10	63.0
124.80	174.0
125.10	180.0
125.80	101.0
127.90	423.0
129.00	186.0
129.80	352.0
130.90	257.0
132.80	335.0
134.90	315.0
137.00	251.0
138.80	77.0
139.60	74.0
140.10	59.0
140.80	1289.0
141.90	218.0
142.90	1197.0
144.00	133.0
145.00	365.0
145.80	137.0
146.80	135.0
147.20	129.0
147.90	366.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

149.10	62.0
150.00	153.0
154.00	83.0
154.90	357.0
156.90	289.0
158.80	170.0
161.00	170.0
169.60	72.0
170.60	197.0
172.00	834.0
174.00	77096.0
175.10	6708.0
176.00	79672.0
177.00	5207.0
178.00	161.0
178.80	75.0
190.70	198.0
191.20	161.0
192.30	70.0
193.00	359.0
194.20	50.0
205.00	64.0
207.10	217.0
249.10	98.0
249.80	75.0
250.90	108.0
265.10	209.0
280.20	177.0
281.10	1829.0
282.20	645.0
282.90	359.0
284.30	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

m/z	Abundance
36.00	1329.0
37.10	6028.0
38.00	5898.0
39.10	2356.0
40.00	279.0
43.20	54.0
44.00	949.0
45.00	1214.0
46.00	142.0
47.00	1487.0
48.00	889.0
49.00	5739.0
50.00	24120.0
51.00	8148.0
52.00	361.0
52.90	73.0
55.00	452.0
56.10	2220.0
57.00	4344.0
58.10	172.0
59.10	58.0
60.00	1405.0
61.00	7175.0
62.00	6891.0
63.00	5237.0
64.00	473.0
65.00	606.0
66.30	117.0
67.00	367.0
68.00	14004.0
69.00	14561.0
70.00	976.0
70.90	56.0
72.00	755.0
73.10	6858.0
74.00	25488.0
75.00	77088.0
76.00	6679.0
77.00	771.0
78.00	638.0
78.90	4902.0
80.00	1421.0
80.90	4597.0
81.90	1193.0
82.90	200.0
86.00	239.0
86.90	5850.0
88.00	5515.0
90.90	664.0
92.00	4089.0
93.00	6674.0
94.00	18240.0
95.00	138112.0
96.10	9428.0
97.00	363.0
103.00	96.0
103.90	805.0
104.90	277.0
106.00	661.0
106.80	136.0
109.70	98.0
110.90	219.0
111.90	89.0
113.10	146.0
114.90	200.0
115.80	439.0
117.00	876.0
117.80	537.0
118.90	1041.0
122.90	62.0
124.00	66.0
124.80	85.0
127.90	411.0
129.00	317.0
130.00	568.0
130.90	238.0
132.70	70.0
134.90	393.0
135.70	61.0
136.90	273.0
138.80	67.0
139.80	186.0
141.00	1612.0
142.10	173.0
143.00	1660.0
144.90	252.0
145.90	394.0
146.90	124.0
148.00	346.0
149.00	75.0
149.90	189.0
153.00	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

153.90	77.0
154.70	233.0
155.10	230.0
157.10	253.0
158.90	212.0
161.00	199.0
170.80	197.0
172.00	858.0
174.00	100056.0
175.00	8468.0
176.00	98000.0
177.00	6818.0
190.90	139.0
192.30	62.0
192.90	282.0
207.20	83.0
248.80	102.0
249.20	111.0
250.90	90.0
265.10	140.0
281.20	1518.0
281.90	338.0
282.20	399.0
283.00	332.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

m/z	Abundance
36.10	817.0
37.00	5125.0
38.00	4437.0
39.00	1587.0
39.90	266.0
43.10	87.0
43.90	760.0
45.00	1059.0
47.10	1107.0
47.90	814.0
49.00	4609.0
50.00	19000.0
51.10	5669.0
52.00	349.0
55.10	345.0
56.10	1496.0
57.10	2780.0
58.00	143.0
60.00	1243.0
61.00	5788.0
62.00	4995.0
63.00	4283.0
64.00	449.0
65.10	458.0
65.80	89.0
66.90	340.0
68.00	11475.0
69.00	11342.0
70.00	961.0
72.10	583.0
73.00	5874.0
74.00	19216.0
75.00	59136.0
76.10	4771.0
76.90	700.0
77.90	560.0
78.90	3384.0
80.00	1052.0
81.00	3707.0
81.90	986.0
82.80	73.0
85.80	340.0
87.00	4419.0
87.90	4667.0
90.90	504.0
92.00	3584.0
93.10	4679.0
94.00	13546.0
95.00	111600.0
96.00	7980.0
97.10	306.0
103.90	557.0
104.90	197.0
105.90	496.0
106.90	133.0
110.00	81.0
110.90	104.0
111.90	73.0
112.80	150.0
114.80	137.0
116.00	532.0
116.90	754.0
117.80	416.0
118.90	689.0
124.00	55.0
125.70	77.0
127.80	356.0
128.90	248.0
129.90	369.0
131.00	192.0
134.90	287.0
136.90	210.0
137.10	210.0
138.90	77.0
139.80	82.0
141.00	1446.0
141.80	209.0
142.90	1342.0
143.80	79.0
145.00	279.0
145.80	124.0
146.70	88.0
147.10	72.0
148.00	324.0
148.90	118.0
149.90	221.0
151.70	59.0
153.00	55.0
153.80	62.0
154.90	236.0
156.90	234.0
159.00	202.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

161.00	140.0
170.90	198.0
172.20	780.0
174.00	83568.0
175.00	6868.0
176.00	87464.0
177.00	5601.0
178.00	254.0
191.00	105.0
192.90	128.0
248.80	54.0
265.10	73.0
281.10	747.0
282.00	210.0
283.10	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483