
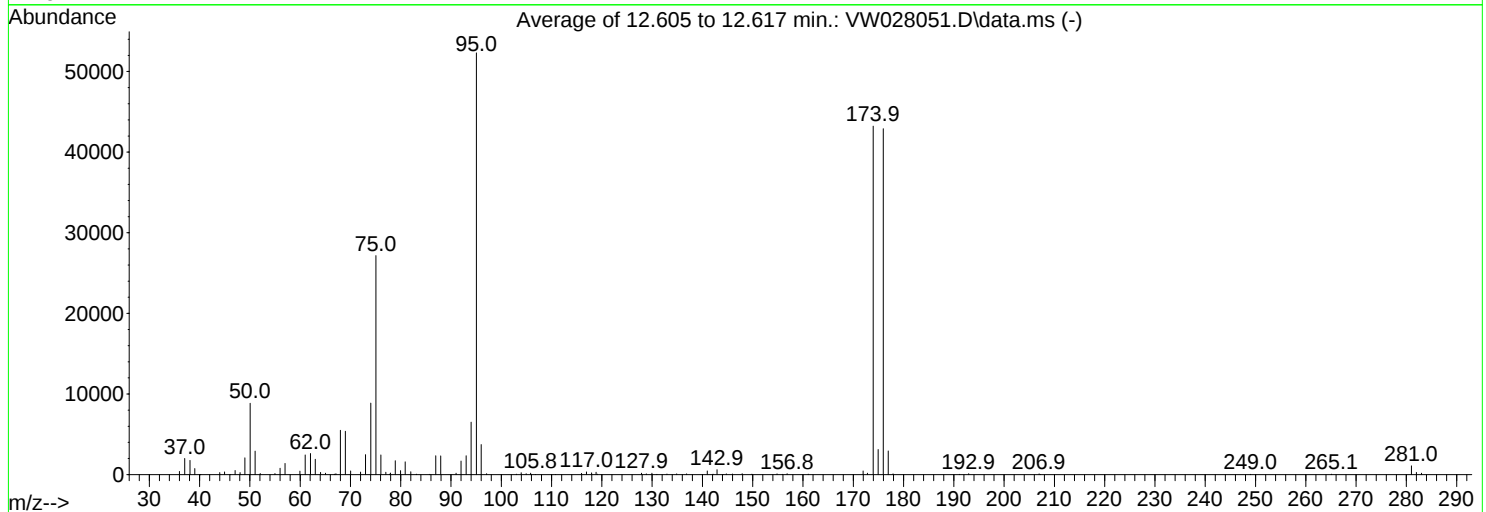


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022324\
Data File : VW028051.D
Acq On : 23 Feb 2024 12:20
Operator : SY/MD
Sample : BFB441
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB441

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Fri Feb 23 22:35:45 2024

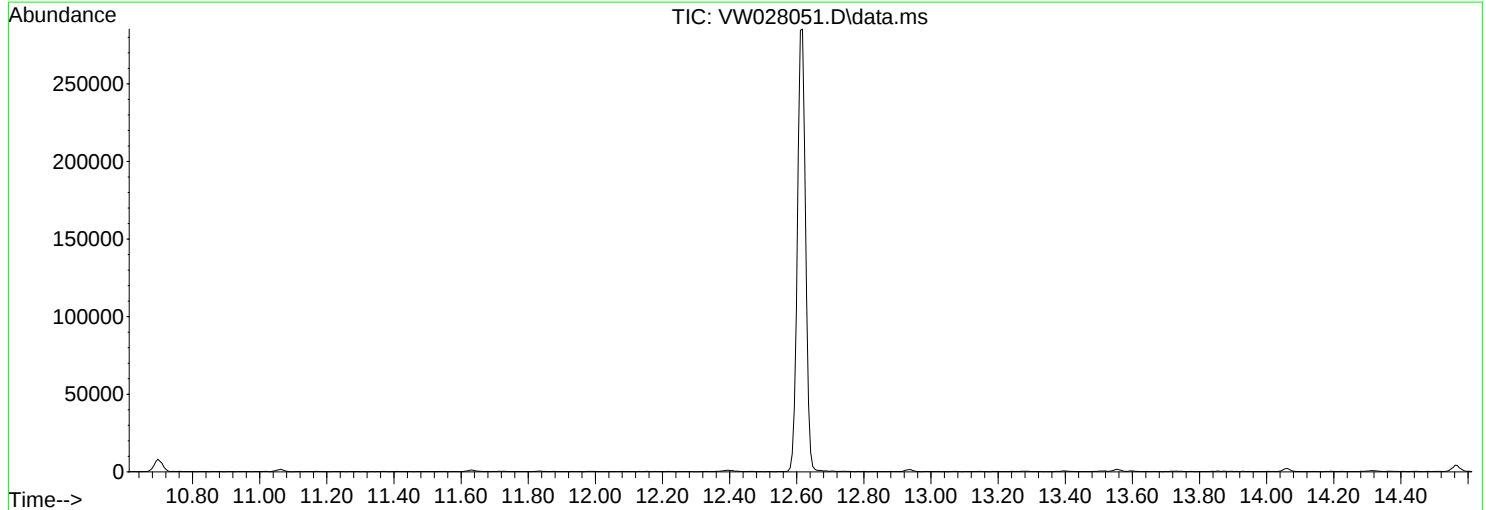

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	8844	PASS
75	95	30	80	51.9	27171	PASS
95	95	100	100	100.0	52315	PASS
96	95	5	9	7.1	3739	PASS
173	174	0.00	2	0.4	179	PASS
174	95	50	120	82.6	43232	PASS
175	174	5	9	7.2	3119	PASS
176	174	95	101	99.2	42896	PASS
177	176	5	9	6.8	2928	PASS

m/z	Abundance
40.10	109.0
44.00	96.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	336.0
37.00	1798.0
38.10	1578.0
39.00	669.0
40.10	127.0
44.00	299.0
45.00	236.0
47.00	459.0
48.00	248.0
49.00	1679.0
50.10	7648.0
51.10	2569.0
52.00	132.0
55.00	126.0
56.00	624.0
57.00	1121.0
59.90	420.0
61.00	1958.0
62.00	2224.0
63.00	1607.0
64.00	248.0
65.10	179.0
66.80	159.0
68.00	4460.0
69.00	4477.0
70.00	466.0
72.10	197.0
73.00	2152.0
74.00	7403.0
75.00	21976.0
76.10	2078.0
77.10	263.0
77.80	171.0
78.90	1476.0
80.00	324.0
80.90	1387.0
82.00	257.0
83.10	72.0
87.00	1853.0
88.00	2152.0
91.00	137.0
92.00	1558.0
93.00	1990.0
94.00	5024.0
95.00	43688.0
96.00	2773.0
97.10	125.0
103.10	58.0
103.90	220.0
105.10	78.0
105.90	138.0
116.00	121.0
116.90	284.0
118.00	206.0
118.80	197.0
119.10	214.0
128.00	145.0
128.90	82.0
129.90	103.0
133.10	82.0
135.00	87.0
136.90	86.0
141.00	414.0
142.90	503.0
144.70	113.0
145.90	66.0
147.80	119.0
149.90	67.0
154.80	113.0
157.00	58.0
172.00	337.0
174.00	32560.0
174.90	2524.0
175.90	30536.0
176.90	2017.0
177.90	53.0
191.10	82.0
193.00	140.0
207.00	89.0
249.00	125.0
265.10	176.0
281.00	1616.0
282.00	399.0
283.00	269.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	395.0
37.10	1962.0
38.10	1972.0
39.10	851.0
40.00	114.0
44.00	385.0
45.00	406.0
47.10	705.0
48.00	244.0
49.00	2417.0
50.00	10012.0
51.00	3273.0
52.10	139.0
55.00	154.0
56.00	955.0
57.00	1534.0
60.00	480.0
61.00	2727.0
62.10	2880.0
63.00	2150.0
64.00	328.0
65.00	209.0
67.10	156.0
68.00	5877.0
69.00	6012.0
70.00	468.0
72.00	402.0
73.00	2565.0
74.00	9739.0
75.10	30016.0
76.00	2658.0
77.00	264.0
78.00	344.0
78.90	1831.0
79.90	545.0
80.90	1668.0
82.00	424.0
83.10	57.0
87.00	2632.0
88.00	2234.0
91.00	166.0
92.00	1902.0
93.00	2531.0
94.00	7228.0
95.00	58456.0
96.00	4216.0
97.10	101.0
103.00	73.0
103.90	218.0
104.90	127.0
105.90	180.0
110.80	54.0
116.00	147.0
116.90	394.0
117.90	217.0
118.90	369.0
127.90	249.0
128.80	93.0
130.00	179.0
130.90	55.0
132.90	71.0
134.80	113.0
136.80	125.0
140.90	499.0
142.10	94.0
142.90	744.0
144.10	56.0
144.80	90.0
145.90	76.0
147.90	83.0
149.90	57.0
154.90	81.0
155.90	71.0
156.80	145.0
161.10	56.0
171.90	476.0
174.00	46544.0
175.00	3001.0
176.00	47616.0
176.90	3368.0
177.90	107.0
191.10	53.0
192.90	114.0
206.90	74.0
207.20	76.0
280.90	1095.0
282.00	303.0
283.00	167.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	485.0
37.00	2251.0
38.10	1753.0
39.10	734.0
40.00	108.0
44.00	375.0
44.90	377.0
46.10	59.0
47.00	363.0
48.10	260.0
49.00	2169.0
50.10	8872.0
51.00	2922.0
52.00	170.0
55.00	149.0
56.00	826.0
57.00	1485.0
60.00	434.0
61.00	2636.0
62.00	2784.0
63.00	1985.0
64.10	257.0
65.00	161.0
67.10	179.0
68.00	6127.0
69.00	5629.0
70.10	433.0
71.90	352.0
73.00	2740.0
74.10	9447.0
75.00	29520.0
76.00	2597.0
77.00	363.0
77.90	255.0
78.90	1897.0
80.00	626.0
80.90	1732.0
82.00	408.0
83.10	64.0
85.80	114.0
86.90	2548.0
87.90	2560.0
91.00	217.0
92.00	1621.0
93.00	2511.0
94.00	7270.0
95.10	54800.0
96.00	4228.0
97.10	108.0
102.90	54.0
104.00	274.0
104.90	135.0
105.80	203.0
106.80	88.0
115.90	222.0
117.00	343.0
117.90	254.0
118.80	348.0
127.80	166.0
128.80	102.0
130.00	277.0
131.00	96.0
132.90	74.0
134.90	123.0
136.90	101.0
141.00	471.0
142.10	75.0
142.90	590.0
144.80	69.0
146.00	92.0
148.00	164.0
149.80	58.0
154.90	128.0
155.90	64.0
156.80	130.0
161.00	99.0
171.90	536.0
172.80	538.0
173.90	50592.0
175.00	3831.0
175.90	50536.0
177.00	3398.0
177.90	115.0
193.00	83.0
206.90	106.0
281.10	559.0
282.00	118.0
283.10	128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441