


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022423\
Data File : VW025369.D
Acq On : 24 Feb 2023 12:16
Operator : SY/MD
Sample : VSTDCCC025EC
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 27 00:39:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM02223SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 22 21:27:06 2023
Response via : Initial Calibration

Reviewed By :
Supervised By :

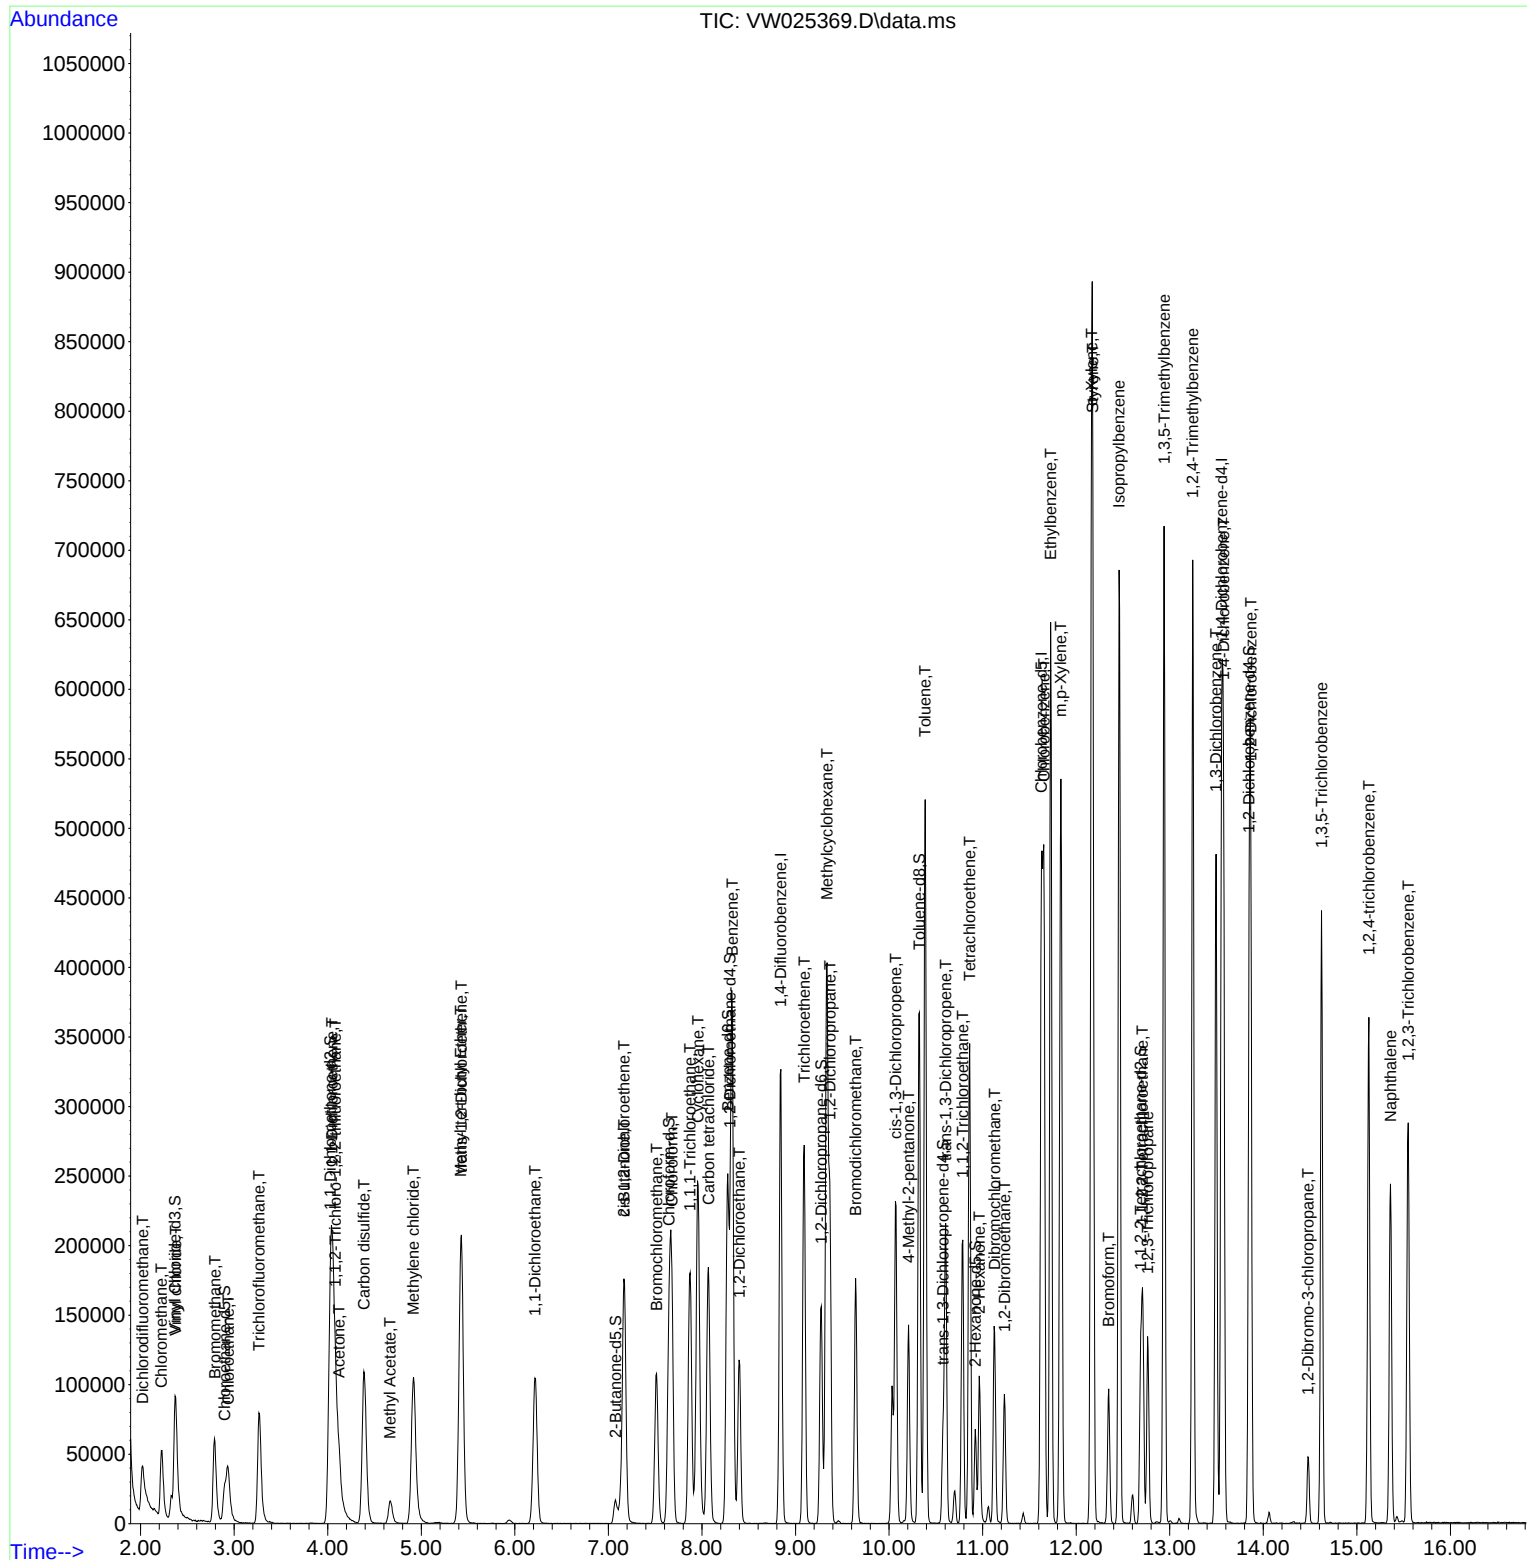




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022423\
Data File : VW025369.D
Acq On : 24 Feb 2023 12:16
Operator : SY/MD
Sample : VSTDCCC025EC
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 27 00:39:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 22 21:27:06 2023
Response via : Initial Calibration

Reviewed By :
Supervised By :

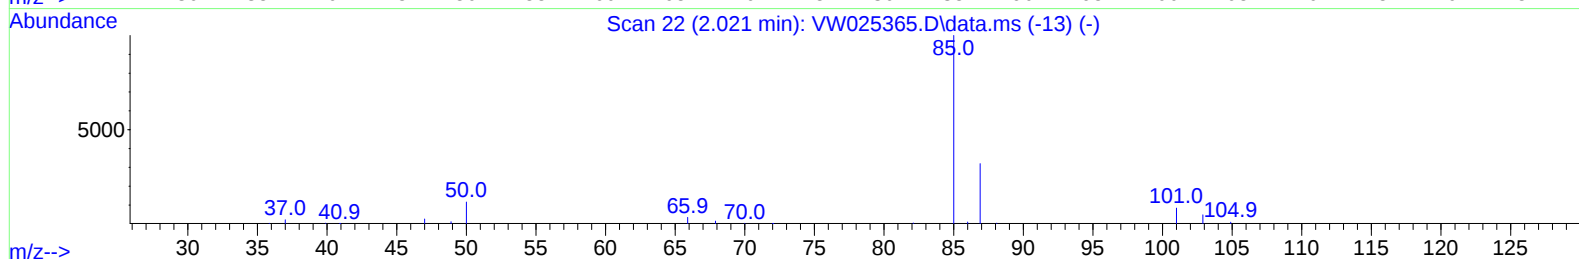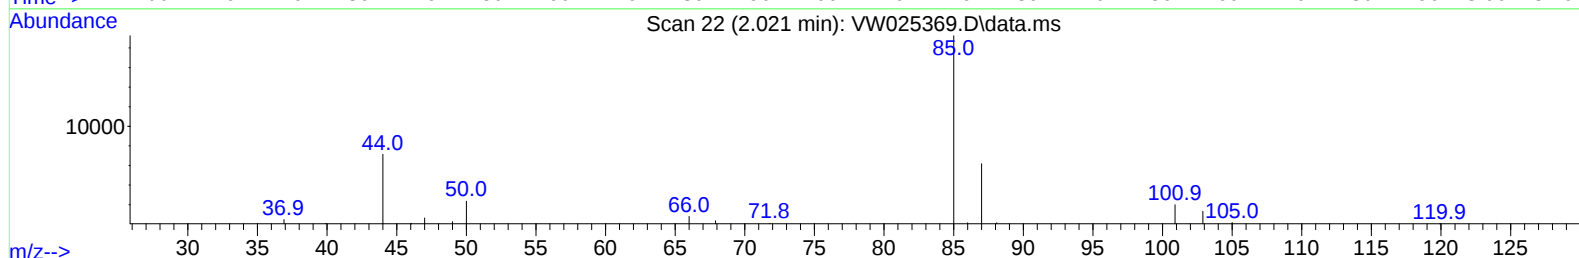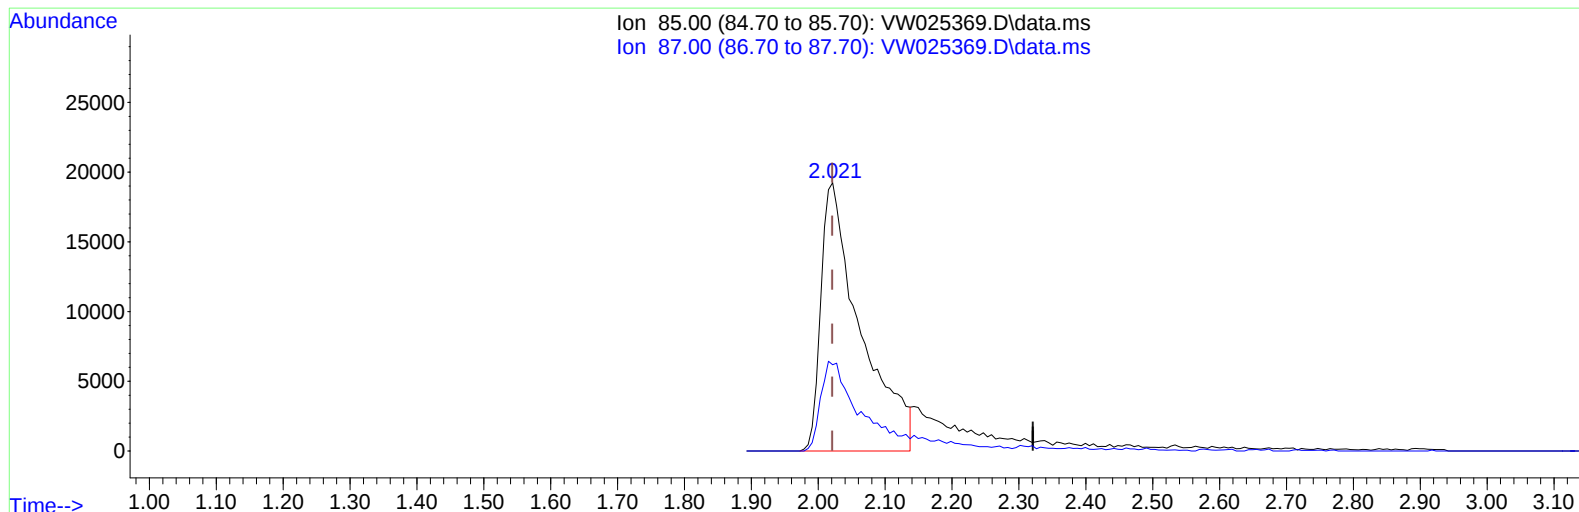

TIC: VW025369.D\data.ms

(2) Dichlorodifluoromethane (T)

2.021min (+ 0.000) 23.53 ug/L

response 78975

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	25.70	22.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022423\
Data File : VW025369.D
Acq On : 24 Feb 2023 12:16
Operator : SY/MD
Sample : VSTDCCC025EC
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 27 00:39:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 22 21:27:06 2023
Response via : Initial Calibration

Reviewed By :
Supervised By :

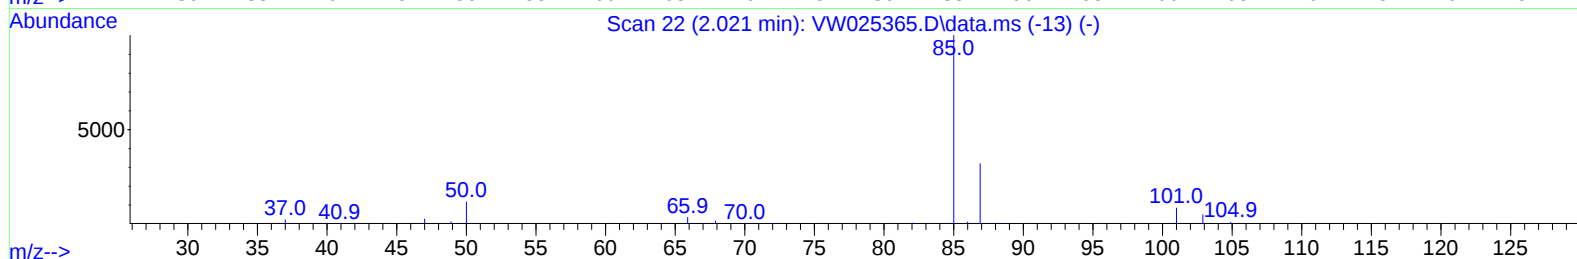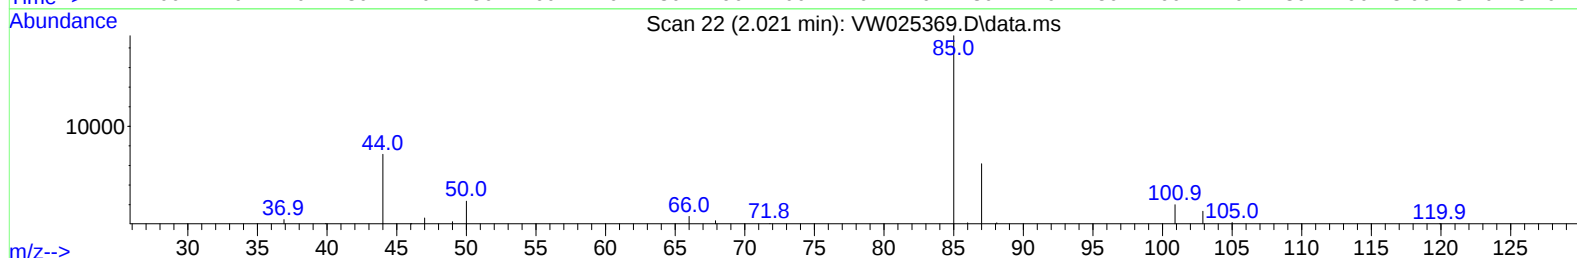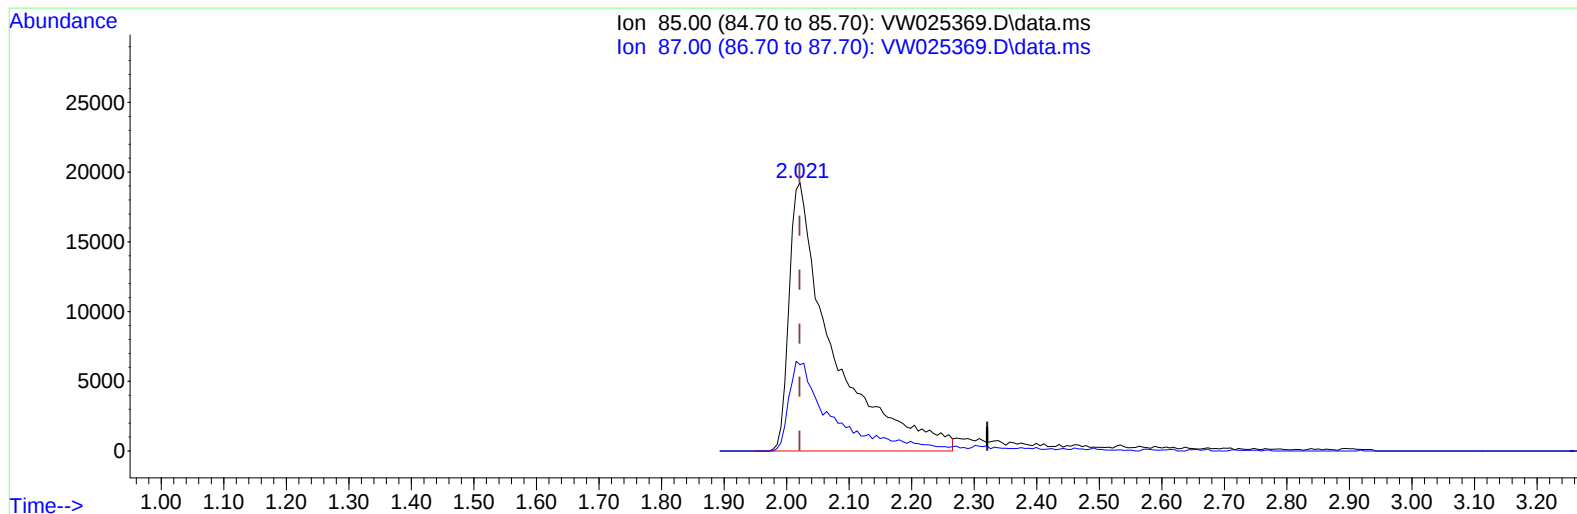

TIC: VW025369.D\data.ms

(2) Dichlorodifluoromethane (T)

2.021min (+ 0.000) 27.66 ug/L m

response 92832

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	25.70	19.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022423\
 Data File : VW025369.D
 Acq On : 24 Feb 2023 12:16
 Operator : SY/MD
 Sample : VSTDCCC025EC
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 27 00:39:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 22 21:27:06 2023
 Response via : Initial Calibration

Reviewed By :
 Supervised By :

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	267341	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	238753	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120559	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	51462	22.738	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.960%
7) Chloroethane-d5	2.899	69	38470	23.055	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	4.027	63	145621	24.788	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	99.160%
21) 2-Butanone-d5	7.075	46	27017	52.621	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.240%
24) Chloroform-d	7.648	84	139723	27.245	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	109.000%
26) 1,2-Dichloroethane-d4	8.301	65	74945	28.171	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.680%
32) Benzene-d6	8.276	84	258745	25.573	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.280%
36) 1,2-Dichloropropane-d6	9.276	67	70252	24.743	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.960%
41) Toluene-d8	10.325	98	247678	26.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.040%
43) trans-1,3-Dichloroprop...	10.575	79	34145	26.397	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	105.600%
47) 2-Hexanone-d5	10.922	63	22678	54.756	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.520%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	56510	26.586	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	77110	25.183	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.720%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.021	85	92832m	27.661	ug/L	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022423\
 Data File : VW025369.D
 Acq On : 24 Feb 2023 12:16
 Operator : SY/MD
 Sample : VSTDCCC025EC
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Manual IntegrationsAPPROVED

Quant Time: Feb 27 00:39:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022223SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 22 21:27:06 2023
 Response via : Initial Calibration

Reviewed By :
 Supervised By :

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	8.398	62	114830	25.493	ug/L	98
29) Cyclohexane	7.959	56	138842	23.101	ug/L	98
30) 1,1,1-Trichloroethane	7.874	97	154827	25.034	ug/L	98
31) Carbon tetrachloride	8.069	117	144264	24.782	ug/L	99
33) Benzene	8.325	78	341623	23.401	ug/L	100
34) Trichloroethene	9.093	95	94945	23.288	ug/L	98
35) Methylcyclohexane	9.337	83	168176	23.539	ug/L	99
37) 1,2-Dichloropropane	9.368	63	80911	22.913	ug/L	99
38) Bromodichloromethane	9.642	83	114943	23.997	ug/L	97
39) cis-1,3-Dichloropropene	10.069	75	137014	23.715	ug/L	98
40) 4-Methyl-2-pentanone	10.209	43	84993	47.312	ug/L	99
42) Toluene	10.386	91	372204	23.683	ug/L	98
44) trans-1,3-Dichloropropene	10.605	75	120677	24.848	ug/L	99
45) 1,1,2-Trichloroethane	10.788	97	63089	23.953	ug/L	94
46) Tetrachloroethene	10.861	164	73739	23.952	ug/L	98
48) 2-Hexanone	10.965	43	62696	46.759	ug/L	98
49) Dibromochloromethane	11.129	129	75270	24.740	ug/L	97
50) 1,2-Dibromoethane	11.233	107	59905	23.725	ug/L	94
51) Chlorobenzene	11.654	112	238722	23.652	ug/L	98
52) Ethylbenzene	11.727	91	439048	24.108	ug/L	98
53) m,p-Xylene	11.837	106	168372	24.332	ug/L	99
54) o-Xylene	12.166	106	155908	24.372	ug/L	98
55) Styrene	12.178	104	267210	24.561	ug/L	98
57) 1,1,2,2-Tetrachloroethane	12.708	83	70783	23.541	ug/L	100
59) Bromoform	12.349	173	42831	23.731	ug/L	99
60) Isopropylbenzene	12.459	105	444360	22.535	ug/L	100
61) 1,2,3-Trichloropropane	12.763	75	53399	22.356	ug/L	99
62) 1,3,5-Trimethylbenzene	12.940	105	374316	23.637	ug/L	99
63) 1,2,4-Trimethylbenzene	13.245	105	361636	24.125	ug/L	99
64) 1,3-Dichlorobenzene	13.495	146	181719	23.568	ug/L	96
65) 1,4-Dichlorobenzene	13.574	146	186315	24.103	ug/L	95
67) 1,2-Dichlorobenzene	13.867	146	165419	23.395	ug/L	98
68) 1,2-Dibromo-3-chloropr...	14.476	75	13577	24.600	ug/L	97
69) 1,3,5-Trichlorobenzene	14.623	180	127116	24.086	ug/L	97
70)						