
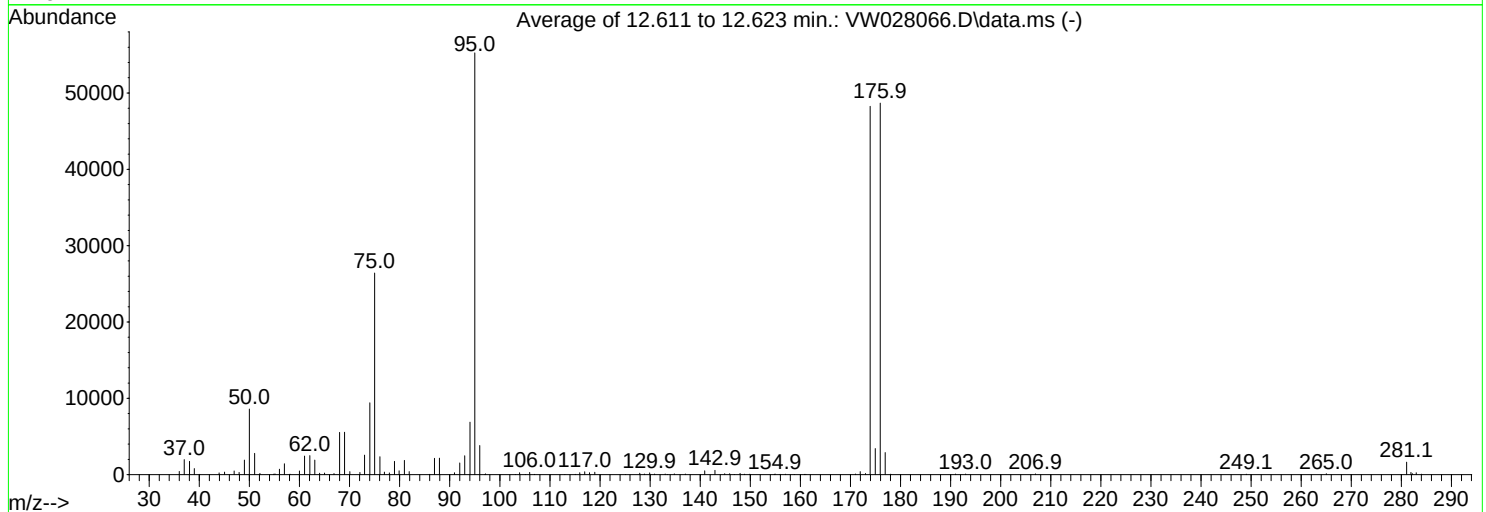


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022724\
Data File : VW028066.D
Acq On : 27 Feb 2024 08:43
Operator : SY/MD
Sample : BFB443
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB443

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Wed Feb 28 00:18:10 2024

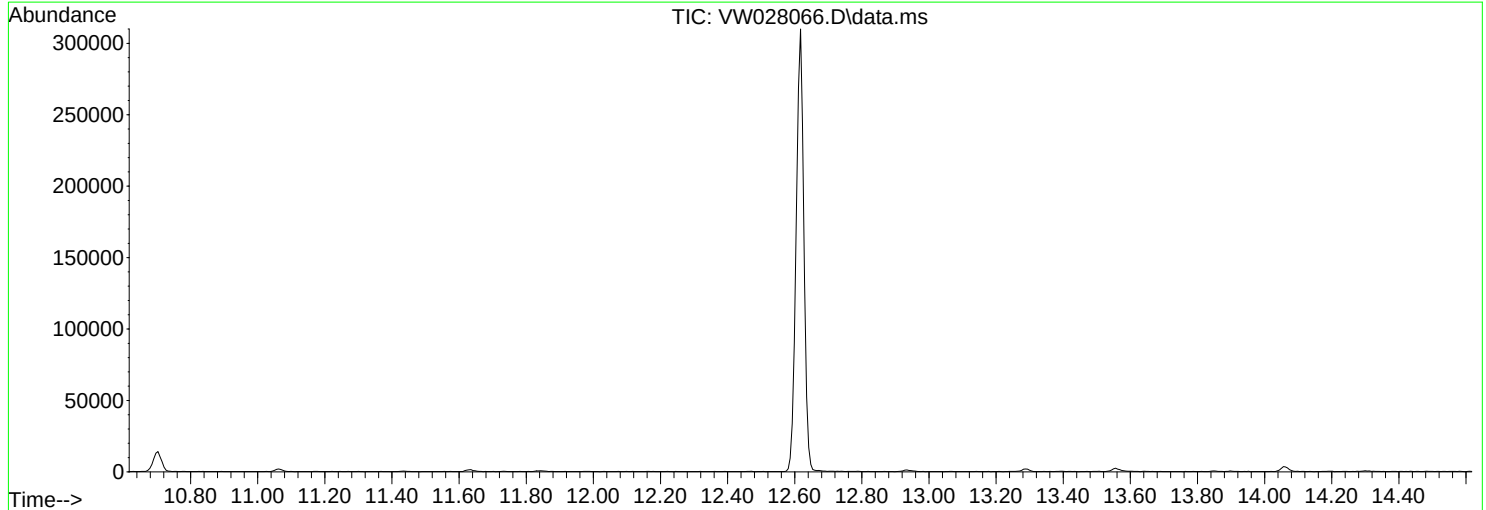

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	8604	PASS
75	95	30	80	47.8	26405	PASS
95	95	100	100	100.0	55264	PASS
96	95	5	9	6.9	3809	PASS
173	174	0.00	2	0.3	139	PASS
174	95	50	120	87.3	48264	PASS
175	174	5	9	7.1	3425	PASS
176	174	95	101	100.8	48669	PASS
177	176	5	9	6.0	2904	PASS

m/z	Abundance
40.00	136.0
44.00	103.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

m/z	Abundance
36.00	524.0
37.00	2132.0
38.00	1912.0
39.00	884.0
39.90	151.0
44.00	361.0
45.10	390.0
47.00	568.0
47.90	309.0
49.00	1991.0
50.00	9202.0
51.00	3129.0
52.10	138.0
54.90	76.0
55.10	77.0
56.00	734.0
57.00	1414.0
58.10	87.0
60.00	489.0
61.00	2718.0
62.10	2669.0
63.00	2040.0
64.00	219.0
65.10	285.0
66.90	167.0
68.00	5558.0
69.00	5747.0
70.00	426.0
72.00	275.0
73.00	2612.0
74.10	9787.0
75.00	27440.0
76.00	2467.0
77.00	306.0
78.00	234.0
78.90	1834.0
79.90	550.0
80.90	1903.0
81.90	500.0
85.90	89.0
86.90	1995.0
88.00	2046.0
90.90	224.0
92.00	1478.0
93.00	2679.0
94.00	6993.0
95.00	53040.0
96.00	3938.0
97.00	85.0
104.00	249.0
106.00	289.0
106.90	62.0
115.00	68.0
116.00	212.0
117.00	349.0
117.90	205.0
118.90	329.0
127.90	165.0
128.90	136.0
129.90	266.0
130.90	96.0
133.00	183.0
134.80	71.0
137.10	78.0
140.90	412.0
143.00	593.0
144.90	172.0
145.90	150.0
147.90	153.0
148.90	76.0
154.80	132.0
158.80	63.0
160.80	54.0
161.20	67.0
171.00	93.0
171.90	362.0
174.00	41952.0
174.90	3212.0
175.90	45880.0
177.00	2567.0
178.00	141.0
191.00	165.0
193.00	183.0
207.00	218.0
249.10	107.0
265.00	259.0
281.00	2707.0
281.90	666.0
282.90	428.0
284.10	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

m/z	Abundance
36.00	405.0
37.00	2222.0
38.10	2030.0
39.00	857.0
39.90	210.0
44.00	335.0
45.00	392.0
46.90	488.0
48.00	349.0
49.00	2088.0
50.00	9439.0
51.10	2932.0
52.10	194.0
55.00	163.0
56.00	756.0
57.00	1691.0
58.10	93.0
60.00	573.0
61.00	2656.0
62.00	2662.0
63.10	1971.0
64.00	207.0
65.00	163.0
66.80	148.0
68.00	6473.0
69.00	6294.0
70.10	413.0
72.10	353.0
73.00	2922.0
74.00	10407.0
75.00	30408.0
76.10	2552.0
77.00	419.0
78.00	262.0
78.90	2060.0
79.90	506.0
81.00	2235.0
82.00	426.0
86.00	67.0
87.00	2491.0
88.00	2539.0
91.00	342.0
92.00	1669.0
93.00	2764.0
94.00	8247.0
95.00	62248.0
96.00	4488.0
97.20	100.0
103.90	281.0
105.80	350.0
106.90	66.0
113.00	69.0
115.10	52.0
115.90	299.0
116.90	431.0
117.90	264.0
119.00	338.0
125.10	56.0
128.00	193.0
128.80	107.0
129.90	262.0
130.90	78.0
133.00	57.0
133.50	70.0
134.90	114.0
137.10	102.0
140.90	585.0
143.00	648.0
144.90	131.0
145.90	151.0
146.80	53.0
148.00	212.0
148.90	78.0
149.90	63.0
155.00	136.0
155.90	60.0
157.00	102.0
161.00	57.0
171.00	88.0
172.00	484.0
173.90	55128.0
175.00	3600.0
176.00	55200.0
176.90	3436.0
178.10	80.0
191.00	99.0
193.00	87.0
206.80	110.0
249.00	92.0
265.10	65.0
281.10	1688.0
282.20	381.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

283.00284.00

243.057.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443

m/z	Abundance
36.00	308.0
37.00	1553.0
38.00	1295.0
39.00	644.0
40.10	126.0
43.90	295.0
45.00	210.0
47.00	391.0
47.90	258.0
49.00	1659.0
50.00	7172.0
51.10	2317.0
52.10	153.0
54.80	93.0
55.20	89.0
56.00	665.0
57.00	1189.0
60.00	418.0
61.00	1938.0
62.00	2131.0
63.00	1687.0
64.00	156.0
64.90	159.0
67.00	152.0
68.00	4577.0
69.00	4637.0
70.00	351.0
72.10	225.0
73.00	2171.0
74.00	8044.0
75.00	21368.0
76.00	2018.0
76.90	311.0
77.90	172.0
79.00	1311.0
79.90	477.0
80.90	1455.0
81.80	289.0
87.00	1954.0
87.90	1886.0
90.90	219.0
92.00	1424.0
93.00	1980.0
94.10	5384.0
95.00	50504.0
96.00	3000.0
97.10	204.0
103.10	55.0
103.90	197.0
105.10	52.0
106.00	244.0
116.00	241.0
117.00	378.0
117.90	270.0
118.90	259.0
127.90	206.0
129.90	195.0
130.90	95.0
134.90	152.0
136.90	83.0
140.90	498.0
142.90	478.0
145.00	66.0
145.90	77.0
148.00	110.0
148.80	63.0
149.90	98.0
154.90	125.0
156.00	64.0
157.00	75.0
160.90	72.0
171.00	78.0
172.00	354.0
173.00	418.0
173.90	47712.0
175.00	3462.0
175.90	44928.0
176.90	2709.0
265.00	70.0
281.00	489.0
282.00	196.0
282.90	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB443