
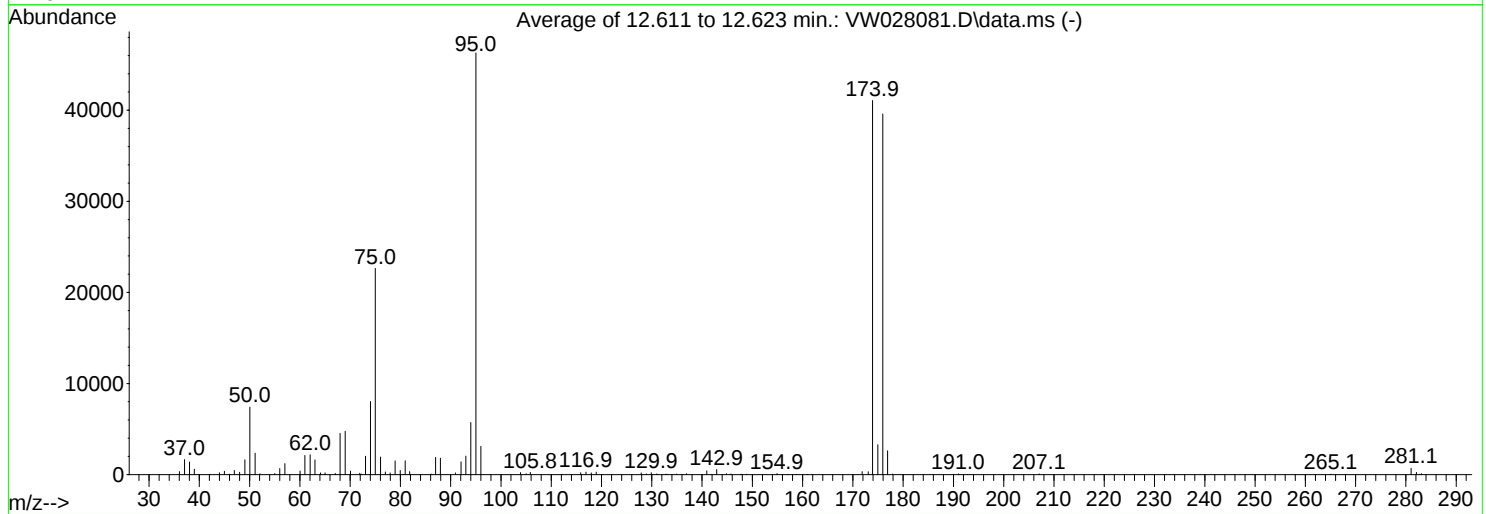


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022924\
Data File : VW028081.D
Acq On : 29 Feb 2024 09:39
Operator : SY/MD
Sample : BFB445
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB445

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Title : SFAM01.0
Last Update : Fri Mar 01 00:41:29 2024

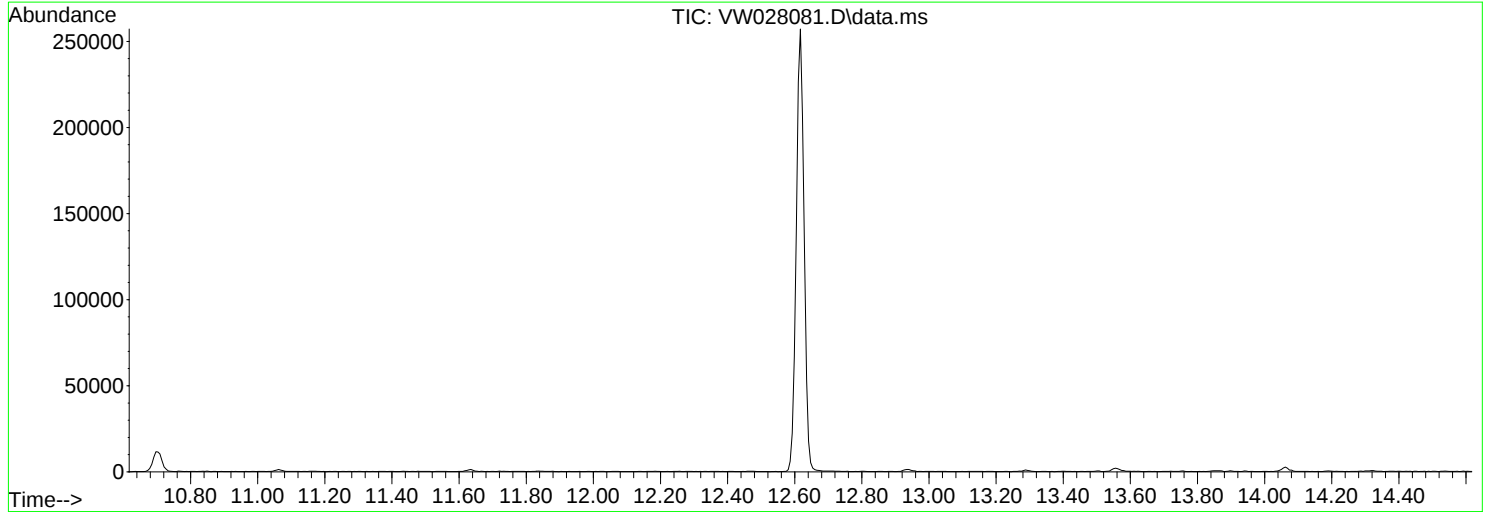

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	7406	PASS
75	95	30	80	48.9	22635	PASS
95	95	100	100	100.0	46296	PASS
96	95	5	9	6.7	3111	PASS
173	174	0.00	2	0.8	317	PASS
174	95	50	120	88.7	41059	PASS
175	174	5	9	8.0	3290	PASS
176	174	95	101	96.4	39592	PASS
177	176	5	9	6.6	2613	PASS

m/z	Abundance
40.00	149.0
43.90	111.0

Instrument :
MSVOA_W
ClientSampleId :
BFB445

m/z	Abundance
36.10	325.0
37.00	1845.0
38.10	1475.0
39.00	656.0
40.00	150.0
44.00	274.0
45.00	405.0
46.00	84.0
47.00	334.0
48.00	335.0
49.00	1820.0
50.10	7889.0
51.10	2499.0
52.00	125.0
55.10	141.0
56.00	698.0
57.00	1167.0
60.10	451.0
61.00	2148.0
62.10	2297.0
63.00	1527.0
64.10	201.0
65.00	197.0
67.10	188.0
68.00	4529.0
69.00	5007.0
70.10	436.0
71.90	307.0
73.00	2118.0
74.10	8325.0
75.00	22960.0
76.10	2095.0
76.90	355.0
77.90	177.0
79.00	1535.0
80.00	451.0
80.90	1660.0
81.90	382.0
85.90	119.0
87.00	1773.0
88.00	2026.0
91.00	188.0
92.00	1435.0
93.00	1937.0
94.00	5973.0
95.00	44808.0
96.00	3123.0
104.00	237.0
105.00	90.0
105.90	199.0
115.80	229.0
116.90	303.0
118.00	188.0
118.90	244.0
127.90	187.0
128.90	70.0
129.80	207.0
131.00	116.0
132.80	148.0
135.00	88.0
136.90	94.0
141.00	405.0
142.90	553.0
144.90	160.0
145.70	59.0
147.90	77.0
148.90	111.0
155.00	118.0
156.90	52.0
160.90	67.0
171.80	299.0
173.90	39008.0
175.00	3071.0
176.00	36288.0
176.90	2470.0
177.80	82.0
191.00	167.0
192.80	74.0
207.00	100.0
265.10	119.0
281.10	1103.0
282.10	472.0
283.10	228.0

Instrument :
MSVOA_W
ClientSampleId :
BFB445

m/z	Abundance
36.00	409.0
37.00	1673.0
38.00	1496.0
39.00	607.0
40.00	195.0
44.00	417.0
45.00	375.0
46.10	67.0
46.90	585.0
48.00	189.0
49.00	1822.0
50.10	8030.0
51.10	2529.0
52.00	91.0
54.90	139.0
56.00	680.0
57.00	1366.0
60.00	489.0
61.00	2449.0
62.00	2350.0
63.00	1828.0
64.00	280.0
65.00	261.0
67.00	138.0
68.00	5191.0
69.00	5420.0
70.00	391.0
72.20	231.0
73.10	2222.0
74.00	8764.0
75.00	25096.0
76.10	2145.0
77.00	362.0
77.90	205.0
79.00	1729.0
80.00	542.0
81.00	1700.0
81.80	327.0
86.10	100.0
87.00	2152.0
87.90	1735.0
91.00	207.0
92.00	1558.0
93.00	2213.0
94.00	6160.0
95.00	51104.0
96.00	3739.0
103.90	231.0
105.10	114.0
105.80	259.0
115.90	201.0
116.90	307.0
117.90	221.0
119.00	368.0
127.90	243.0
128.90	81.0
129.90	274.0
131.00	98.0
133.00	68.0
134.90	87.0
136.90	150.0
140.90	455.0
141.80	80.0
142.90	559.0
144.80	110.0
145.80	75.0
148.00	110.0
148.90	59.0
154.90	161.0
158.80	79.0
161.00	52.0
171.90	326.0
173.10	473.0
173.90	46424.0
174.90	3540.0
175.90	45976.0
176.90	2835.0
177.80	65.0
191.00	77.0
207.10	92.0
265.10	67.0
281.00	778.0
282.10	177.0
282.80	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB445

m/z	Abundance
36.00	243.0
37.10	1426.0
38.00	1202.0
39.00	526.0
40.00	176.0
44.10	282.0
45.00	312.0
47.00	474.0
48.00	275.0
49.10	1281.0
50.00	6300.0
51.10	2014.0
52.10	88.0
55.00	110.0
56.00	604.0
57.00	1116.0
60.10	296.0
61.00	1720.0
62.00	1868.0
63.00	1471.0
64.20	111.0
65.00	135.0
67.00	87.0
68.00	3903.0
69.00	3849.0
70.10	343.0
71.90	169.0
73.00	1732.0
74.00	7000.0
75.00	19848.0
76.00	1549.0
77.10	197.0
78.00	184.0
78.90	1286.0
79.90	361.0
81.00	1203.0
81.90	299.0
86.10	93.0
87.00	1779.0
87.90	1674.0
90.90	183.0
92.10	1213.0
93.00	1952.0
94.00	5042.0
95.00	42976.0
96.00	2472.0
103.80	242.0
104.90	105.0
105.90	258.0
115.90	189.0
116.90	264.0
117.90	148.0
119.00	219.0
127.90	142.0
128.90	120.0
130.00	134.0
131.10	62.0
133.10	105.0
134.90	60.0
136.80	58.0
140.90	414.0
142.90	598.0
144.90	71.0
145.70	71.0
147.70	128.0
154.80	119.0
157.00	53.0
171.90	359.0
173.00	478.0
173.90	37744.0
175.00	3259.0
175.90	36512.0
176.90	2534.0
177.90	63.0
207.10	58.0
281.00	250.0
282.10	102.0
283.10	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB445