

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022175.D
 Acq On : 04 Mar 2022 13:03
 Operator : SY/VA
 Sample : VW0304SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 05 03:22:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	159803	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	142780	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	70955	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	53435	25.637	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.560%	
7) Chloroethane-d5		2.885	69	36208	22.078	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.320%	
11) 1,1-Dichloroethene-d2		4.019	63	64927	20.341	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.360%	
21) 2-Butanone-d5		7.086	46	14261	40.694	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.380%	
24) Chloroform-d		7.647	84	85712	24.040	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.160%	
26) 1,2-Dichloroethane-d4		8.305	65	42735	23.058	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.240%	
32) Benzene-d6		8.275	84	176794	26.606	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.440%	
36) 1,2-Dichloropropane-d6		9.274	67	47098	25.522	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.080%	
41) Toluene-d8		10.323	98	173967	26.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.320%	
43) trans-1,3-Dichloroprop...		10.579	79	19487	23.816	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.280%	
47) 2-Hexanone-d5		10.927	63	10823	35.659	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.320%	
56) 1,1,2,2-Tetrachloroeth...		12.695	84	34156	21.090	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.360%	
66) 1,2-Dichlorobenzene-d4		13.853	152	59946	26.304	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.200%	
Target Compounds							Qvalue
39) cis-1,3-Dichloropropene		10.037	75	1761	0.719	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022175.D
Acq On : 04 Mar 2022 13:03
Operator : SY/VA
Sample : VW0304SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Mar 05 03:22:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

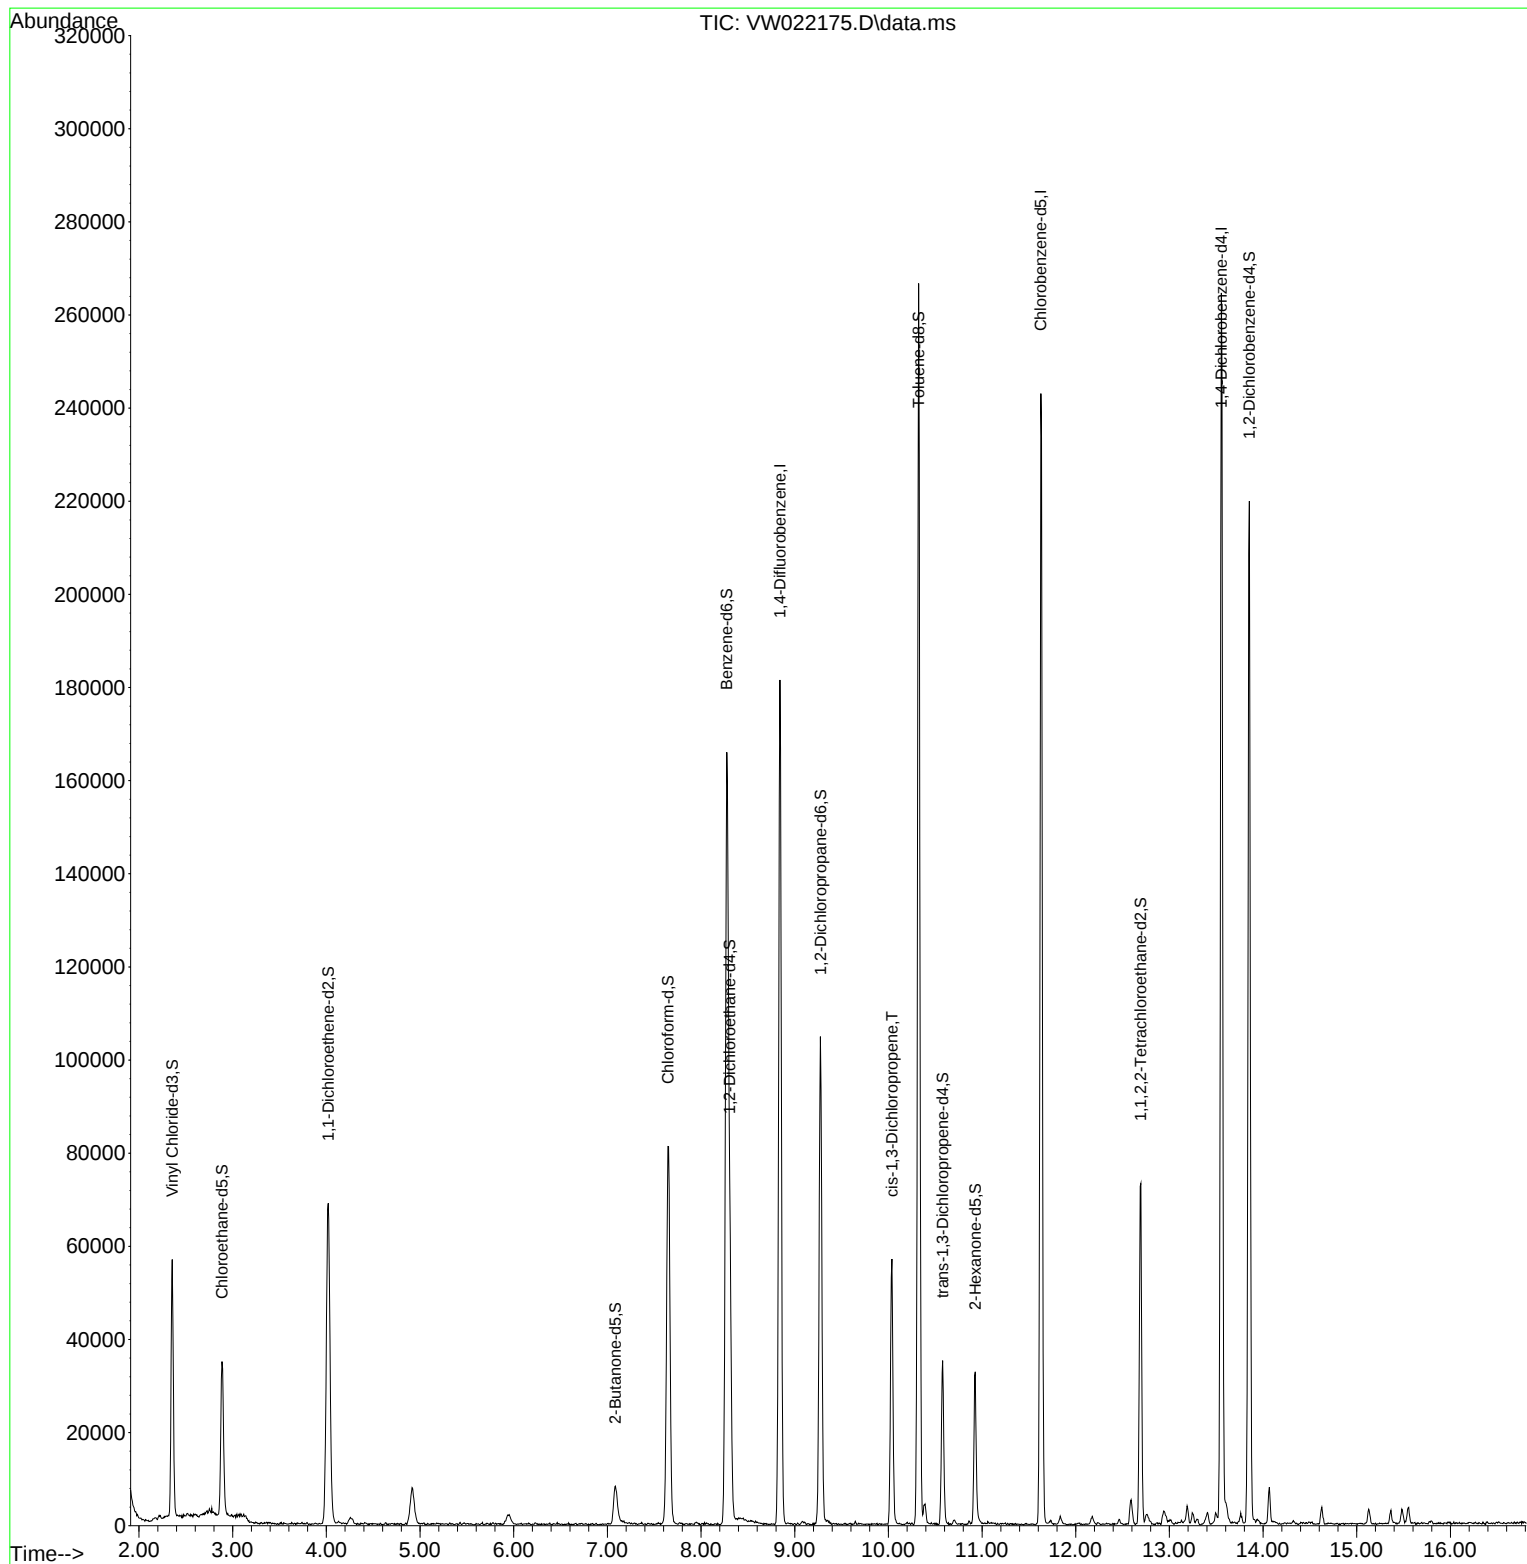

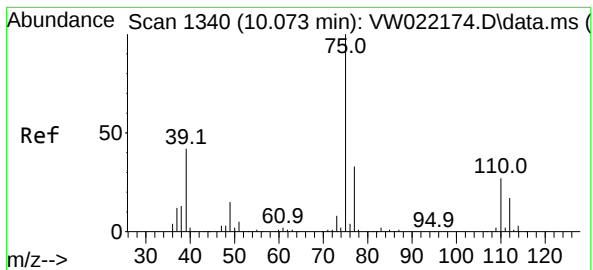

#39
 cis-1,3-Dichloropropene
 Concen: 0.719 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022175.D
 Acq: 04 Mar 2022 13:03

Instrument :
 MSVOA_W
 ClientSampleId :

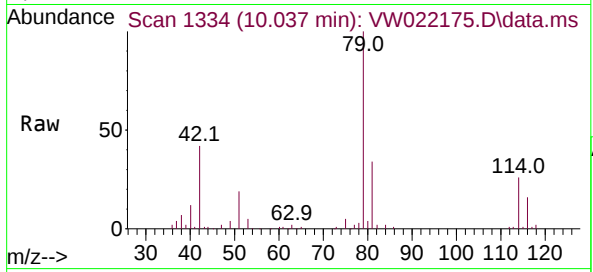

Tgt Ion: 75 Resp: 1761
 Ion Ratio Lower Upper
 75 100
 77 41.8 20.6 38.2#

