

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022176.D
 Acq On : 04 Mar 2022 13:39
 Operator : SY/VA
 Sample : N1775-08
 Misc : 5.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 05 03:22:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	173589	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	162939	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	83280	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	50071	22.115	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.440%
7) Chloroethane-d5	2.885	69	34686	19.471	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.880%
11) 1,1-Dichloroethene-d2	4.019	63	61556	17.754	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.000%
21) 2-Butanone-d5	7.073	46	17874	46.953	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.900%
24) Chloroform-d	7.653	84	88481	22.845	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	8.305	65	47889	23.787	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.160%
32) Benzene-d6	8.274	84	180976	23.865	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.480%
36) 1,2-Dichloropropane-d6	9.274	67	50673	24.062	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.240%
41) Toluene-d8	10.323	98	177183	23.502	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.000%
43) trans-1,3-Dichloroprop...	10.579	79	20953	22.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.760%
47) 2-Hexanone-d5	10.926	63	13924	40.200	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.400%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	40932	22.147	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	64106	23.966	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	1893	0.678	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022176.D
Acq On : 04 Mar 2022 13:39
Operator : SY/VA
Sample : N1775-08
Misc : 5.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Mar 05 03:22:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

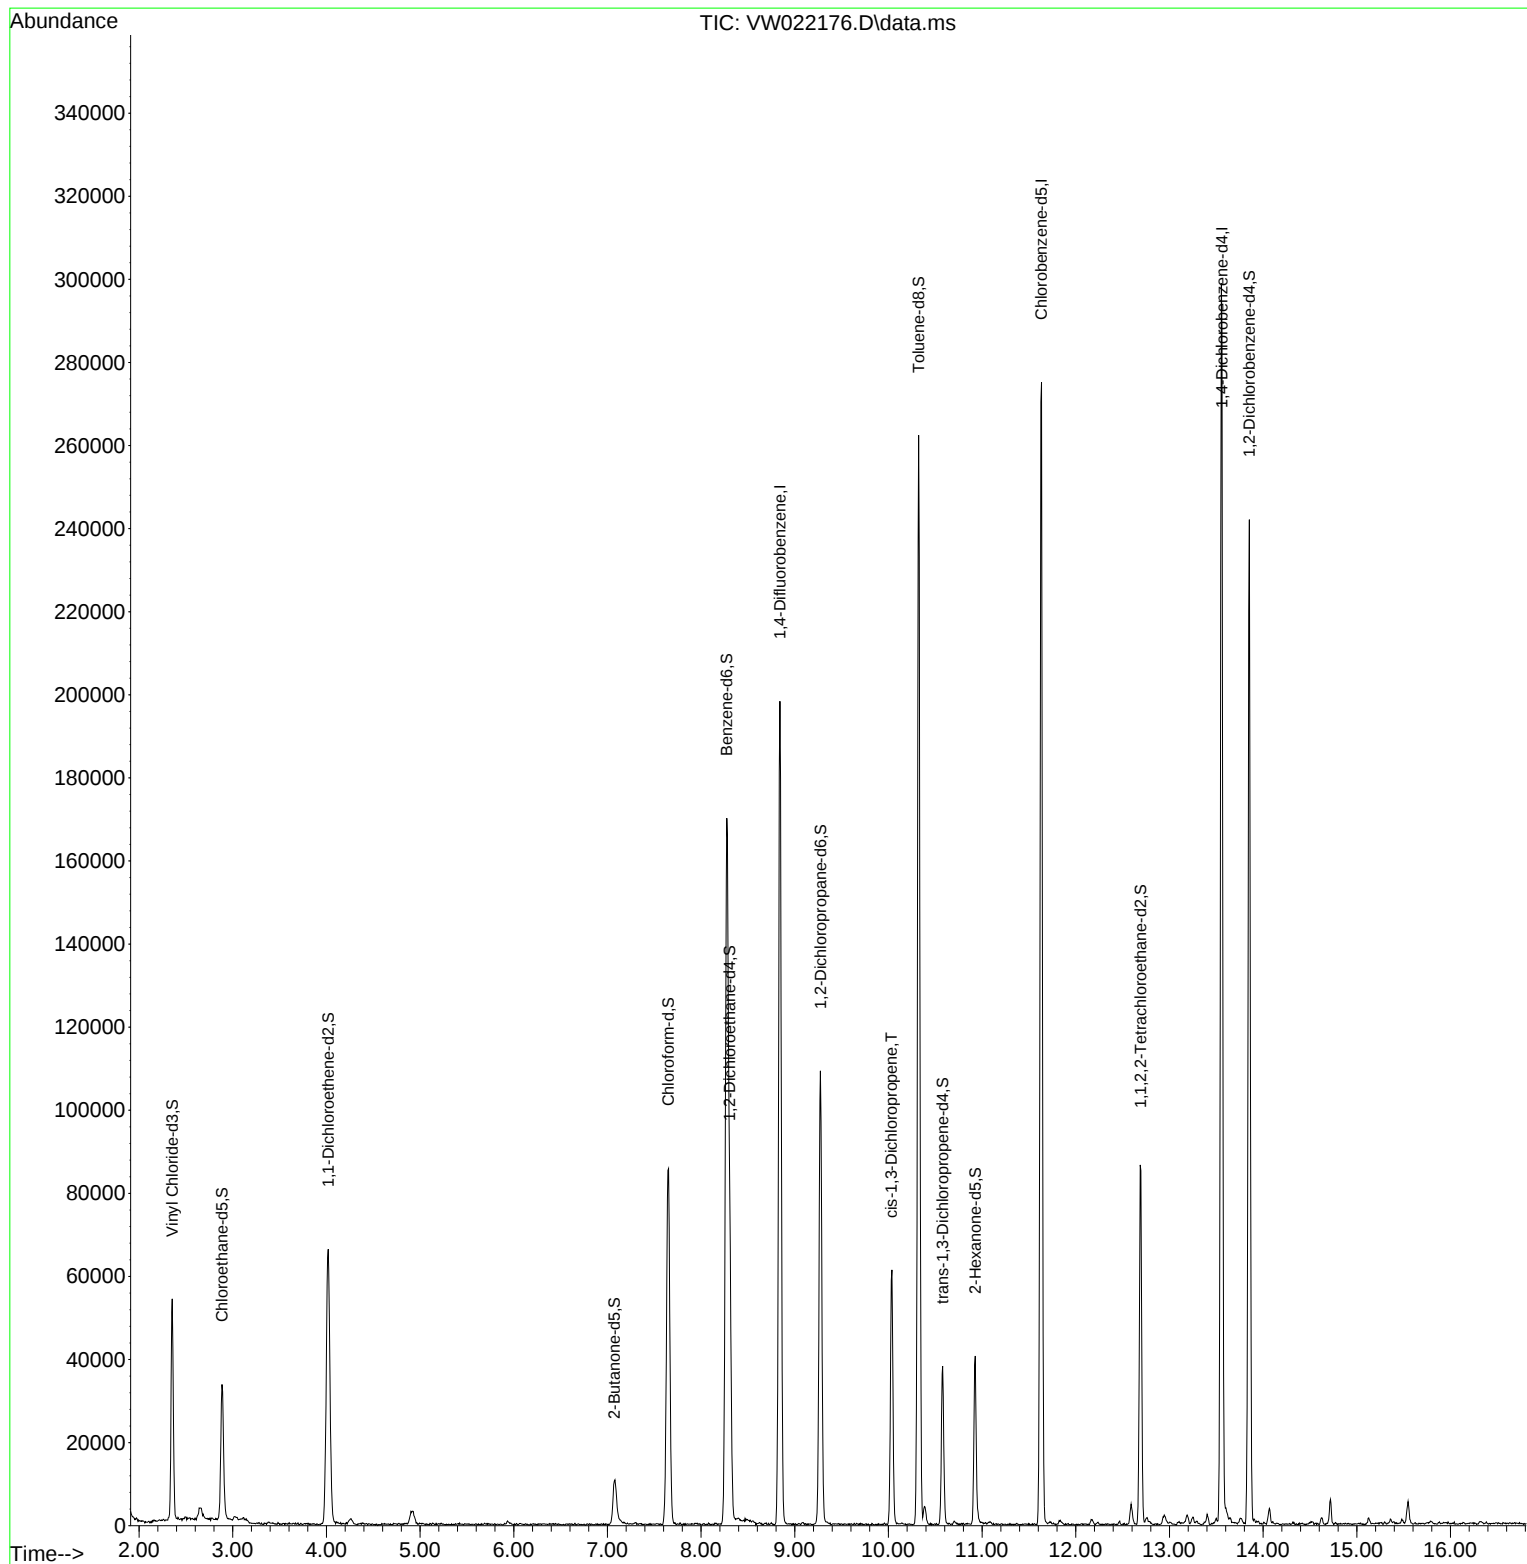

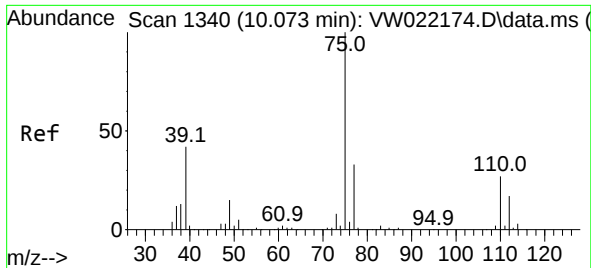

#39
 cis-1,3-Dichloropropene
 Concen: 0.678 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW022176.D
 Acq: 04 Mar 2022 13:39

Instrument :
 MSVOA_W
 ClientSampleId :

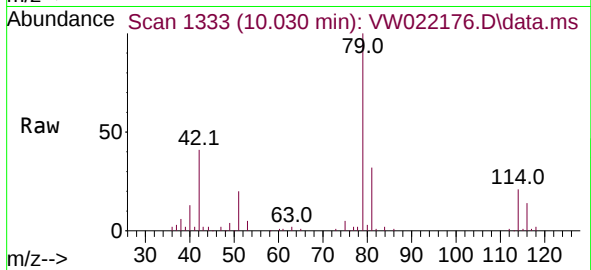

Tgt Ion: 75 Resp: 1893
 Ion Ratio Lower Upper
 75 100
 77 44.6 20.6 38.2#

