

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022177.D
 Acq On : 04 Mar 2022 14:03
 Operator : SY/VA
 Sample : N1733-24
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 05 03:22:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	190866	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	180124	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	85886	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	31471	12.642	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.560%
7) Chloroethane-d5	2.885	69	28319	14.458	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.840%
11) 1,1-Dichloroethene-d2	4.019	63	48262	12.659	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.640%
21) 2-Butanone-d5	7.080	46	24563	58.683	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.360%
24) Chloroform-d	7.653	84	92017	21.608	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.440%
26) 1,2-Dichloroethane-d4	8.305	65	49044	22.156	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.640%
32) Benzene-d6	8.275	84	164768	19.655	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.640%
36) 1,2-Dichloropropane-d6	9.274	67	49695	21.346	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.400%
41) Toluene-d8	10.323	98	155448	18.652	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.600%
43) trans-1,3-Dichloroprop...	10.579	79	19275	18.673	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.680%
47) 2-Hexanone-d5	10.921	63	20723	54.122	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.240%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	47990	23.489	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	62083	22.505	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.040%
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	7.177	96	11605	4.947	ug/L	82
37) 1,2-Dichloropropane	9.274	63	5993	2.950	ug/L	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022177.D
Acq On : 04 Mar 2022 14:03
Operator : SY/VA
Sample : N1733-24
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Mar 05 03:22:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

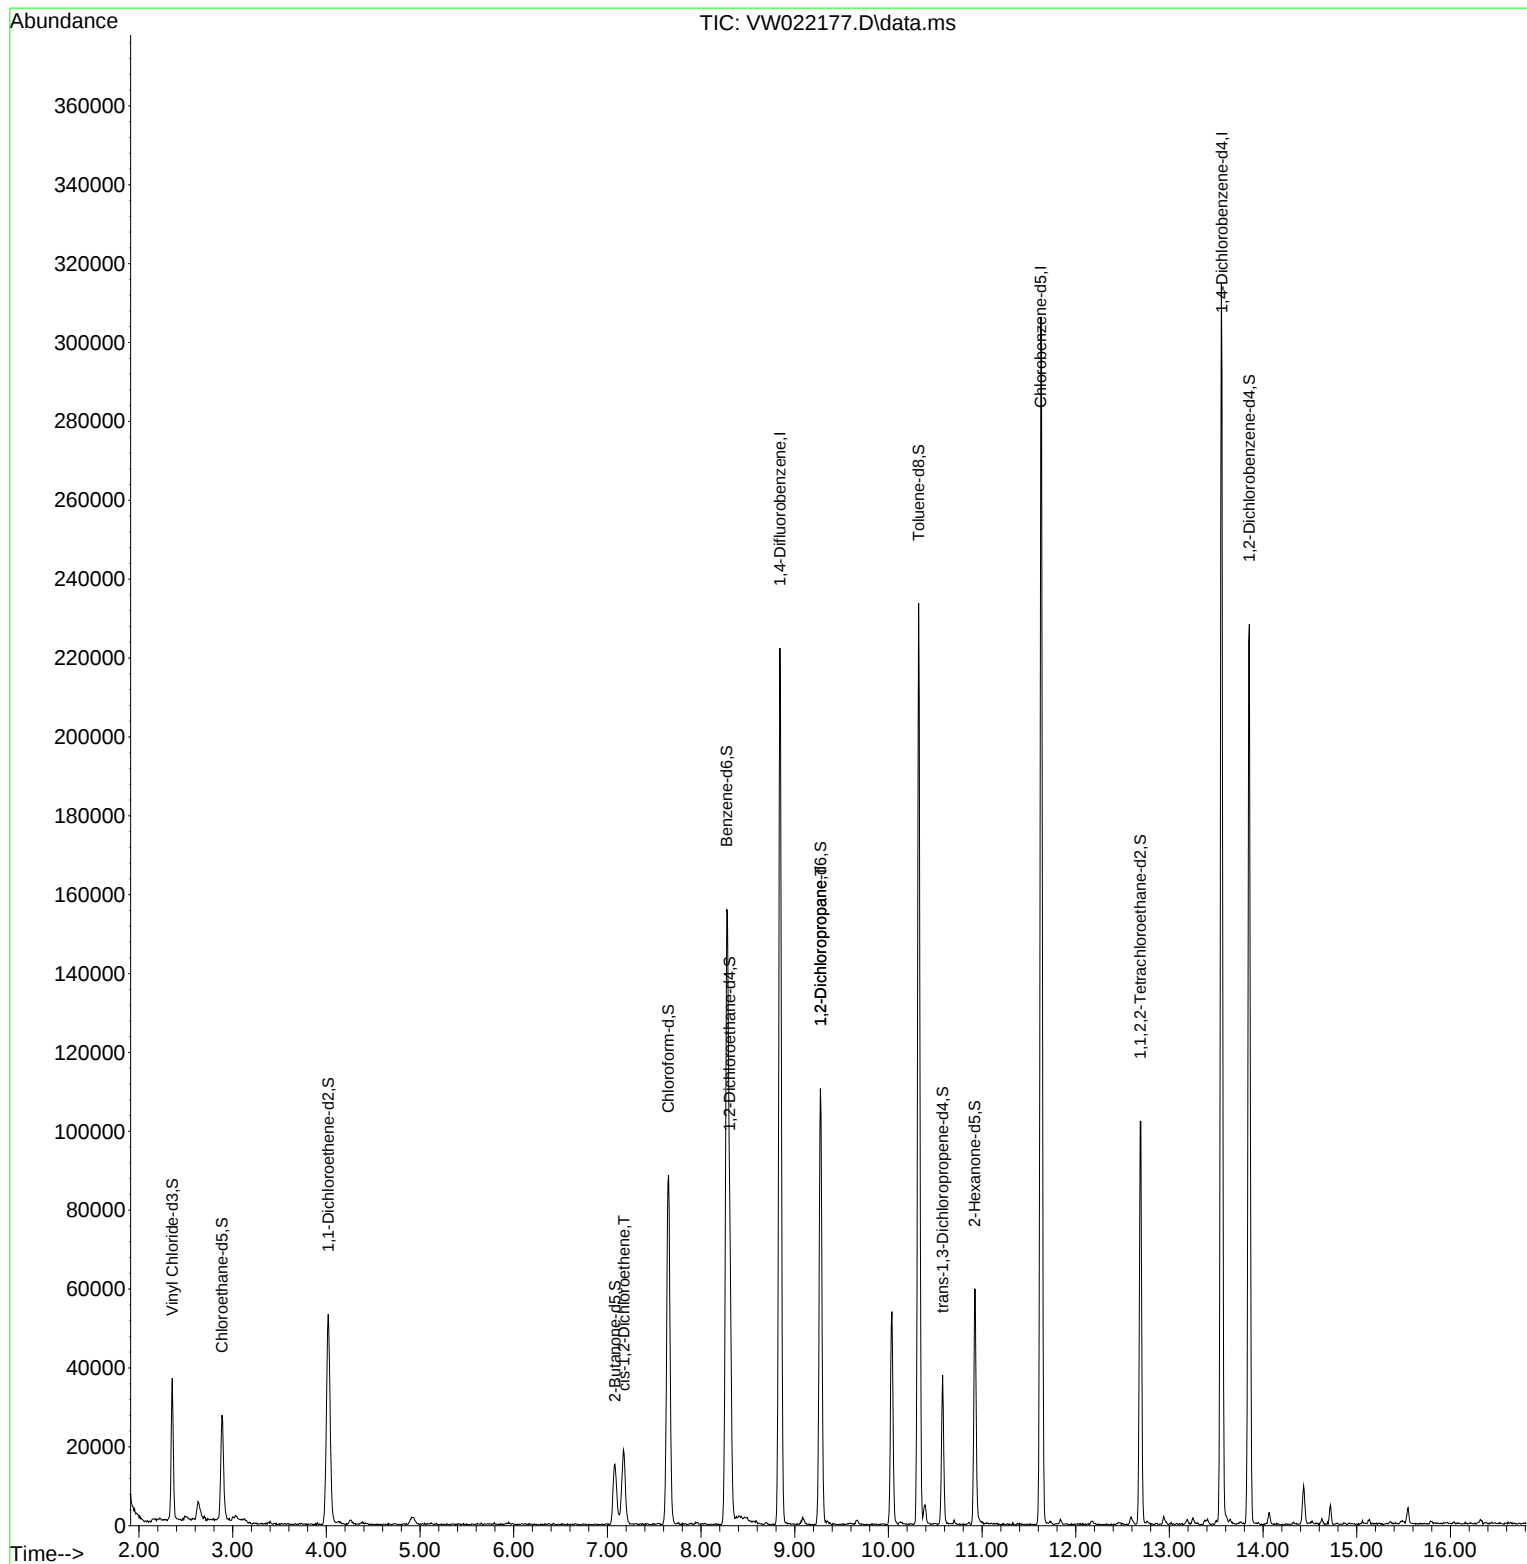



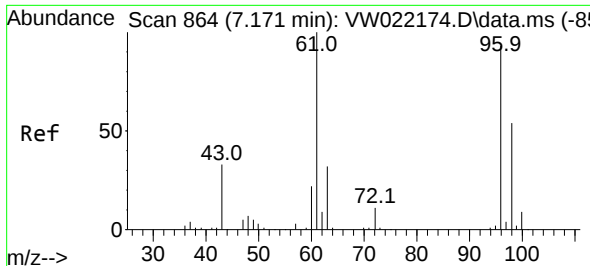


#20
 cis-1,2-Dichloroethene
 Concen: 4.947 ug/L
 RT: 7.177 min Scan# 80
 Delta R.T. 0.006 min
 Lab File: VW022177.D
 Acq: 04 Mar 2022 14:03

Instrument :
 MSVOA_W
 ClientSampleId :

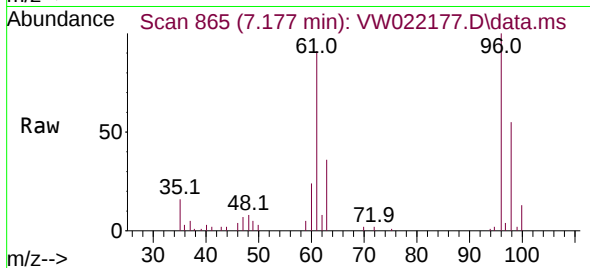

Tgt Ion: 96 Resp: 11605
 Ion Ratio Lower Upper
 96 100
 61 90.8 76.8 142.6
 68 0.0 0.0 0.0

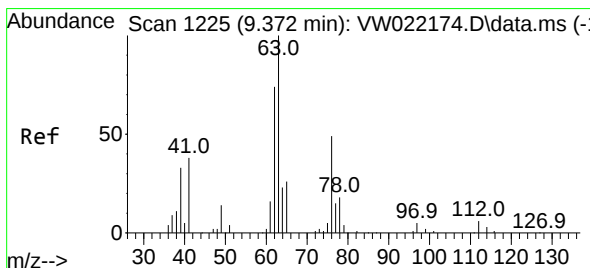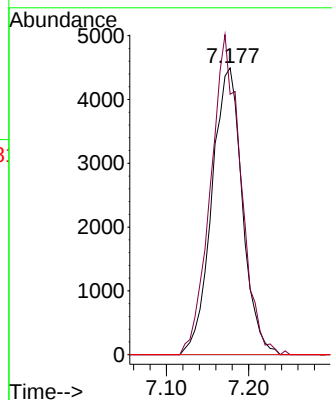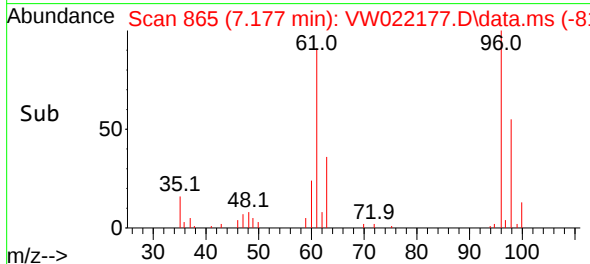

#37
 1,2-Dichloropropane
 Concen: 2.950 ug/L
 RT: 9.274 min Scan# 1209
 Delta R.T. -0.098 min
 Lab File: VW022177.D
 Acq: 04 Mar 2022 14:03

Tgt Ion: 63 Resp: 5993
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.1 6.1#

