

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022181.D
 Acq On : 04 Mar 2022 15:39
 Operator : SY/VA
 Sample : N1775-02
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 05 03:23:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	135325	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	132951	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	66864	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	23425	13.272	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.080%
7) Chloroethane-d5	2.885	69	19331	13.920	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.680%
11) 1,1-Dichloroethene-d2	4.019	63	32783	12.129	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.520%
21) 2-Butanone-d5	7.085	46	24792	83.540	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	167.080%#
24) Chloroform-d	7.652	84	65158	21.581	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.320%
26) 1,2-Dichloroethane-d4	8.305	65	38828	24.740	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.960%
32) Benzene-d6	8.274	84	116414	18.814	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.240%
36) 1,2-Dichloropropane-d6	9.274	67	35720	20.788	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.160%
41) Toluene-d8	10.323	98	107719	17.511	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.040%
43) trans-1,3-Dichloroprop...	10.579	79	15151	19.886	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.560%
47) 2-Hexanone-d5	10.926	63	19799	70.056	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	140.120%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44882	29.762	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	52833	24.601	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.400%
Target Compounds					Qvalue	
13) Acetone	4.135	43	819	3.379	ug/L	68
39) cis-1,3-Dichloropropene	10.030	75	1414	0.620	ug/L #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022181.D
Acq On : 04 Mar 2022 15:39
Operator : SY/VA
Sample : N1775-02
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 05 03:23:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration




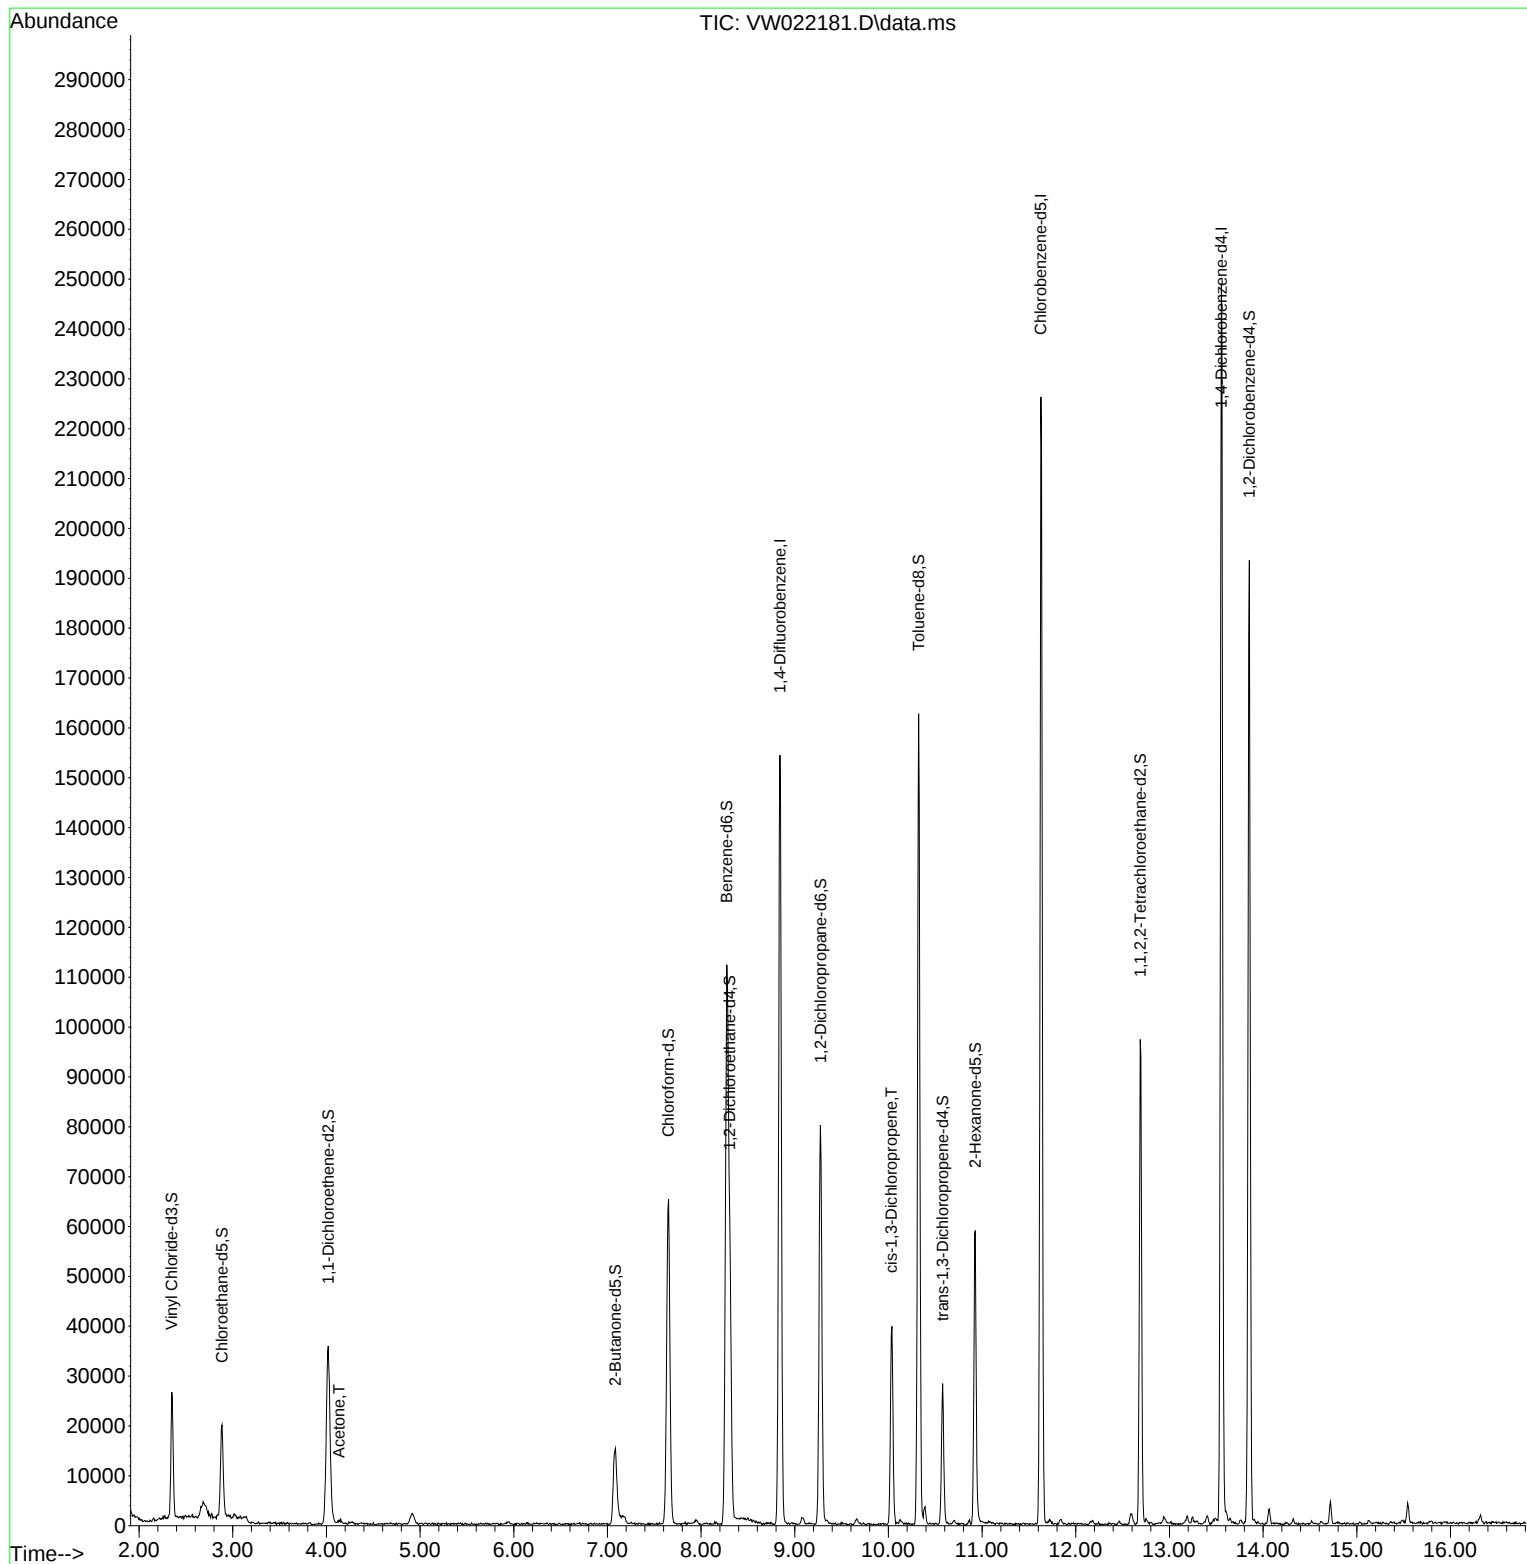


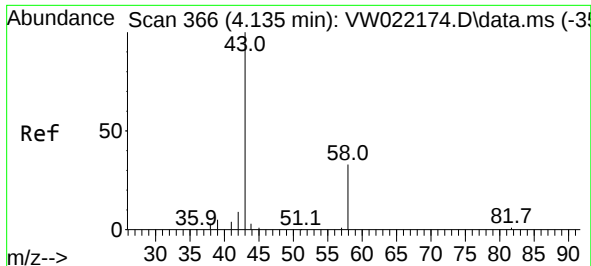

#13
Acetone
Concen: 3.379 ug/L
RT: 4.135 min Scan# 301
Delta R.T. -0.000 min
Lab File: VW022181.D
Acq: 04 Mar 2022 15:39

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 43 Resp: 819
Ion Ratio Lower Upper
43 100
58 16.2 0.0 69.2

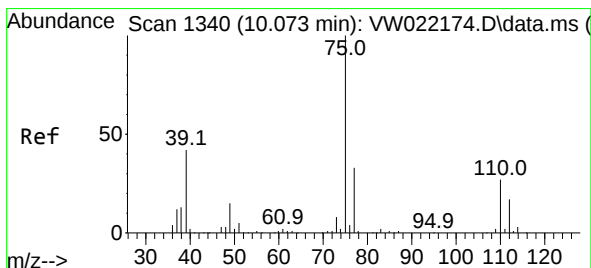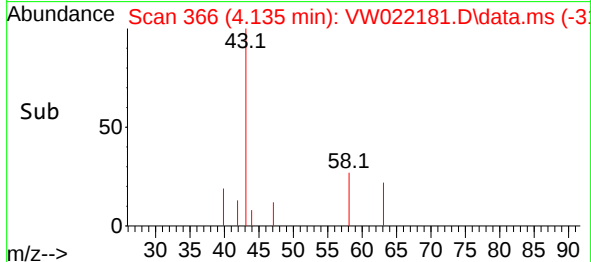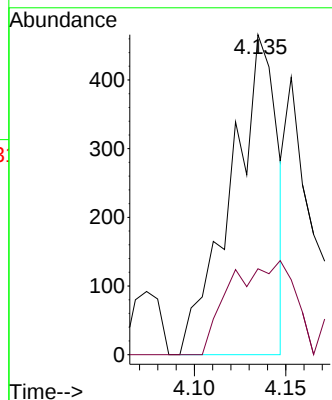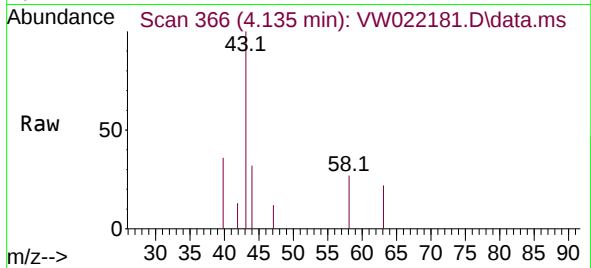

#39
cis-1,3-Dichloropropene
Concen: 0.620 ug/L
RT: 10.030 min Scan# 1333
Delta R.T. -0.043 min
Lab File: VW022181.D
Acq: 04 Mar 2022 15:39

Tgt Ion: 75 Resp: 1414
Ion Ratio Lower Upper
75 100
77 40.3 20.6 38.2#

