

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022184.D
 Acq On : 04 Mar 2022 16:51
 Operator : SY/VA
 Sample : N1733-27
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 05 03:23:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	176950	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	164760	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84384	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	30482	13.207	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.840%
7) Chloroethane-d5	2.885	69	26728	14.719	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.880%
11) 1,1-Dichloroethene-d2	4.013	63	41093	11.627	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.520%
21) 2-Butanone-d5	7.080	46	19170	49.401	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.800%
24) Chloroform-d	7.653	84	79845	20.224	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.880%
26) 1,2-Dichloroethane-d4	8.305	65	41244	20.097	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.400%
32) Benzene-d6	8.275	84	145006	18.911	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.640%
36) 1,2-Dichloropropane-d6	9.274	67	42810	20.104	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.400%
41) Toluene-d8	10.323	98	133838	17.556	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.240%
43) trans-1,3-Dichloroprop...	10.579	79	16868	17.865	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.480%
47) 2-Hexanone-d5	10.927	63	16522	47.174	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.340%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	41561	22.239	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	56173	20.725	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	1378	0.488	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022184.D
Acq On : 04 Mar 2022 16:51
Operator : SY/VA
Sample : N1733-27
Misc : 5.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Mar 05 03:23:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

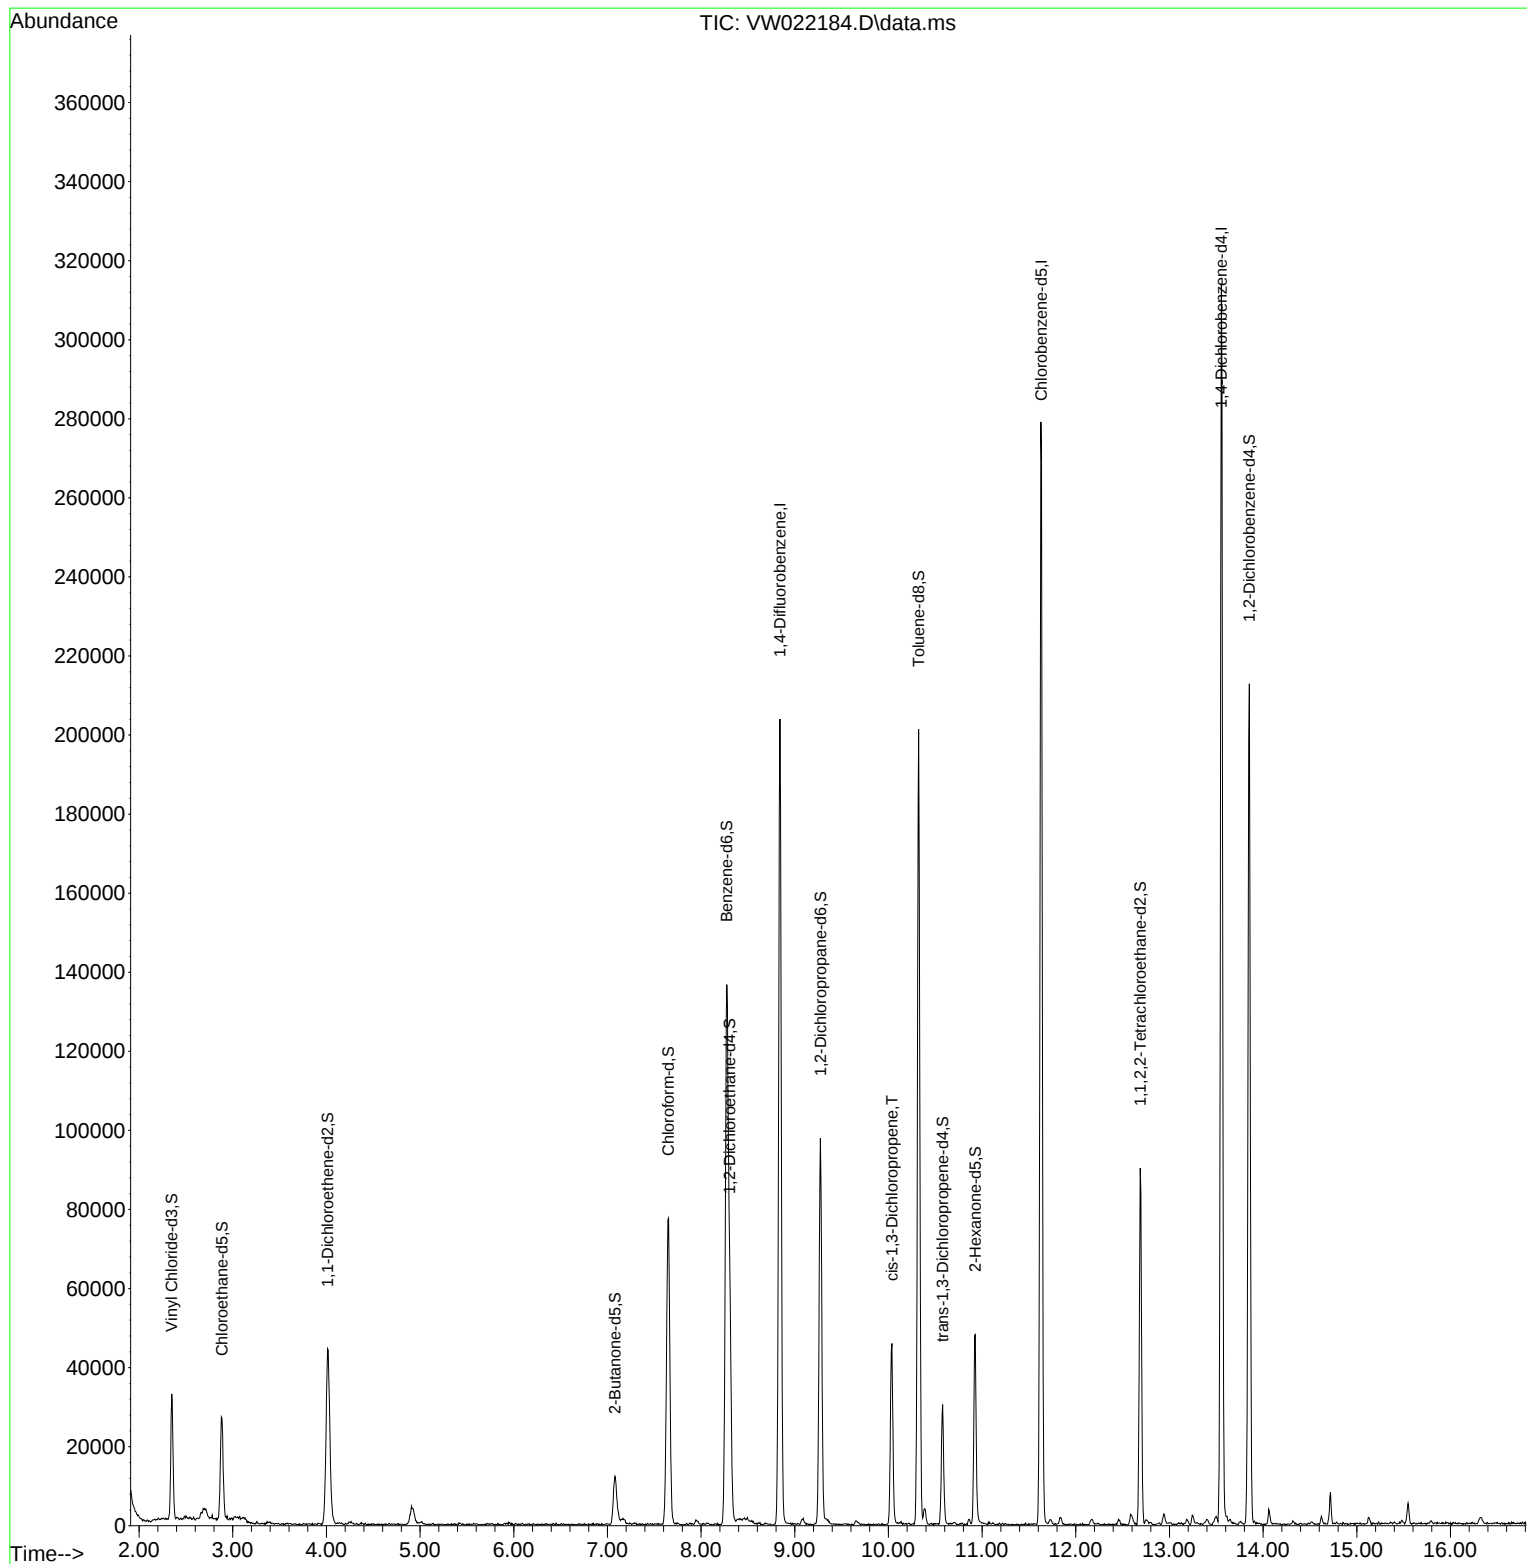

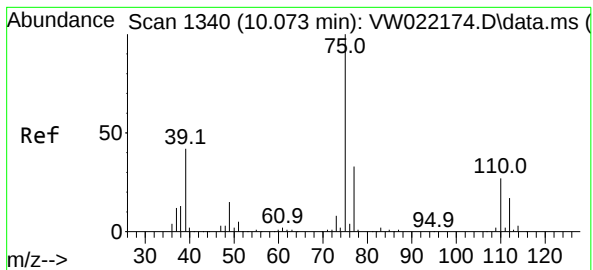

#39
 cis-1,3-Dichloropropene
 Concen: 0.488 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022184.D
 Acq: 04 Mar 2022 16:51

Instrument :
 MSVOA_W
 ClientSampleId :

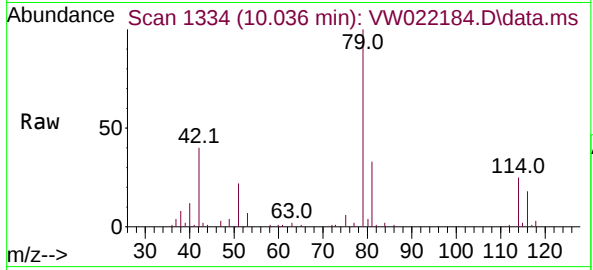

Tgt Ion:	75	Resp:	1378
Ion Ratio	Lower	Upper	
75	100		
77	33.0	20.6	38.2

